

Intensified Tpx3Cam, a fast data-driven optical camera with nanosecond timing resolution for single photon detection in quantum applications

Andrei Nomerotski,^a Matthew Chekhlov,^a Denis Dolzhenko,^a Rene Glazenberg,^b Brianna Farella,^a Michael Keach,^a Ryan Mahon,^a Dmitry Orlov,^b Peter Svihra^{c,d}

^aBrookhaven National Laboratory, Upton NY 11973, USA

^bPhotonis Netherlands BV, 9301 ZR Roden, The Netherlands

^cCzech Technical University, 115 19 Prague, Czech Republic

^dCERN, 1211 Geneva 23, Switzerland

E-mail: anomerotski@bnl.gov

ABSTRACT: We describe a fast data-driven optical camera, Tpx3Cam, with nanosecond scale timing resolution and 80 Mpixel/sec throughput. After the addition of intensifier, the camera is single photon sensitive with quantum efficiency determined primarily by the intensifier photocathode. The single photon performance of the camera was characterized with results on the gain, timing resolution and afterpulsing reported here. The intensified camera was successfully used for measurements in a variety of applications including quantum applications. As an example of such application, which requires simultaneous detection of multiple photons, we describe registration of photon pairs from the spontaneous parametric down-conversion source in a spectrometer. We measured the photon wavelength and timing with respective precisions of 0.15 nm and 3 ns, and also demonstrated that the two photons are anti-correlated in energy.

KEYWORDS: fast imaging, intensifier, Tpx3Cam, spectrometer

¹Corresponding author.

Contents

1	Introduction	1
2	Tpx3Cam fast camera	2
2.1	Intensified Camera	2
2.2	Post-processing	2
3	Characterization of single photon performance	3
3.1	Intensifier gain and signal amplitude	3
3.2	Timing resolution	4
3.3	Afterpulsing	4
3.4	Bias voltage dependence	6
4	Characterization of fast spectrometer based on the camera	6
4.1	Linearity and spectral resolution	6
4.2	Spectral analysis of SPDC source	7
5	Conclusions	7

1 Introduction

The main motivations for fast imaging are studies of fast processes, measuring time of flight and looking for time coincidences of photons. The fast imaging approaches can be generally divided into two types: synchronous and asynchronous. In the former case, a synchronous signal, for example from a pulsed laser, is available, alerting that photons will be coming to the detector so some preparatory operations can be performed. In the latter case, which is more challenging, the measurement must be data driven meaning that a signal can be time stamped independently in each pixel. It is these kinds of cameras that are very attractive for applications where photons are arriving and need to be time stamped at any time in a continuous mode of operation.

A variety of sensing technologies are available for registration of single optical photons, which include approaches with external amplification: iCCD and iCMOS [1–5]; with internal amplification: EMCCDs [6–8] and SPADs [9–13]; and superconductive technologies: SNSPD [14–16] and TES [17, 18]; see comprehensive reviews of the subject in [19–21]. The camera described here, Tpx3Cam, is an intensified hybrid CMOS imager, which is capable of time stamping photon flashes by adding an optical sensor to the Timepix3 readout chip. Single photon sensitivity is provided by an external optical intensifier.

Below we describe different aspects of the camera performance, which are especially important for quantum applications. Firstly, in Section 2 we provide details on the intensified camera. Section 3 discusses several studies important for the single photon detection and Section 4 describes a fast spectrometer used for characterization of a quantum single photon source.

2 Tpx3Cam fast camera

Imaging of single photons in the experiments mentioned here was performed with a time-stamping camera, Tpx3Cam [22–25]. The camera has a silicon optical sensor with high quantum efficiency (QE) [26], which is bump-bonded to Timepix3 [27], an application specific integrated circuit (ASIC) with 256×256 pixels of $55 \times 55 \mu\text{m}^2$. The electronics in each pixel processes the incoming signals to measure their time of arrival (TOA) for hits that cross a predefined threshold, around 600 electrons, with 1.56 ns precision. The information about time-over-threshold (TOT), which is related to the deposited energy in each pixel, is stored together with TOA as time codes. The Timepix3 readout is data driven with pixel deadtime of only $475 \text{ ns} + \text{TOT}$, allowing for multi-hit functionality for each pixel, independently from the other ones, and fast, 80 Mpix/sec, bandwidth [28].

2.1 Intensified Camera

For the single photon sensitive operation, the signal is amplified with addition of CricketTM [29] with integrated image intensifier, power supply and relay optics to project the light flashes from the intensifier output window directly on to the optical sensor in the camera. The image intensifier is a vacuum device comprised of a photocathode followed with a micro-channel plate (MCP) and fast scintillator P47 with risetime of about 7 ns and maximum emission at 430 nm [30]. The quantum efficiency of the camera is determined primarily by the intensifier photocathode with a variety of photocathodes available [24, 29]. As an example, the hi-QE-green photocathode has QE of about 30% in the range of 400 - 480 nm [31]. The MCP in the intensifier had an improved detection efficiency close to 100% [32]. Figure 1 shows schematically the layout of the intensifier and camera, and their photograph.

Similar configurations of the intensified Tpx3Cam were used before for characterization of quantum networks [33, 34], quantum target detection [35, 36], single photon counting and ray tracing [37–40], studies of micromotion in ion traps [41–43], neutron detection [44–46], optical readout of time-projection chamber (TPC) [47] and lifetime imaging [48–50] studies. The Timepix based single photon sensitive cameras with direct registration of MCP electrons with the Timepix ASIC metal pads have also been produced in the past [51].

2.2 Post-processing

Figure 2 shows an example of raw TOT and TOA information for a pair of single photons from a spontaneous parametric down-conversion (SPDC) source registered in Tpx3Cam. As one can see, the photons appear as small groups of hit pixels, so after ordering in time, the pixels are grouped into the "clusters" using a recursive algorithm [23] within a predefined time window, 300 ns. Since all hit pixels measure TOA and TOT independently and provide the position information, it can be used for centroiding to determine the coordinates of single photons. The TOT information is used for the weighted average, giving an estimate of the x, y coordinates for the incoming single photon with improved spatial resolution [48]. The timing of the photon is estimated by using TOA of the pixel with the largest TOT in the cluster.




Figure 1. Left: Schematic layout of the intensified Tpx3Cam camera, not to scale. Right: photograph of the camera with Cricket™.




Figure 2. Raw TOT (left) and TOA (right) values in nanoseconds for pairs of single photon hits in Tpx3Cam.

3 Characterization of single photon performance

3.1 Intensifier gain and signal amplitude

The left part of Figure 3 gives an example of the TOT distribution for the TOT sum over all pixels in the cluster. The distribution is broad due to large fluctuations of the MCP gain, so cannot be used for the photon counting. In this particular case the MCP gain is at maximum of about 10^6 and the TOT distribution peaks at approximately 60,000 electrons. Accounting for the sensor quantum efficiency for the emission spectrum of P47, that means the P47 light flash had about 70,000 photons [26]. We can also see that the distribution for small TOT values has a sharp cutoff near zero due to the Timepix3 threshold. These measurements were performed for the hi-QE-red photocathode [29].

For the measurements described here and also in Sections 3.3 and 3.4, we used the dark counts of a hi-QE-red intensifier. The total dark count rate was about 80 kHz distributed uniformly across the photocathode. This rate is entirely due to the thermal photoelectrons from the photocathode. After going through the detection chain (MCP-P47-Tpx3Cam), these signals look exactly the same and have same properties as signals from the single photons [26].




Figure 3. Left: time-over-threshold (TOT) distribution. Right: distribution of number of pixels in cluster.

The right part of Figure 3 shows the number of pixels in clusters. The maximum of the distribution is at seven pixels. The sub-peak at four pixels is explained by the symmetry of 2×2 pixels square shape.

3.2 Timing resolution

Timing resolution is a critical parameter for many applications. The response of the linear discriminator used in Timepix3 has a time lag, which is dependent on the signal amplitude and can be as large as 100 ns for small signals near the threshold. To account for it and achieve the best possible resolution, a TOT correction must be applied [52, 53]. The left part of Figure 4 shows two instances of TOT correction for the same camera taken at different times as a function of TOT value. These measurements were performed with the same hi-QE-red intensifier as in Section 3.1.




Figure 4. Left: Two instances of TOT correction for the same camera taken at different times; Right: Time difference distribution for a pair of simultaneous photons from SPDC source after the TOT correction.

The right part of Figure 4 shows the time difference distribution for pairs of photons from a SPDC source, which produce simultaneous pairs of photons, after the TOT correction. The time resolution (rms) per photon, assuming equal contributions for two photons in the pair, is $3.3/\sqrt{2} = 2.4$ ns, a typical value achievable after the correction. It was shown that the Timepix3 timing resolution can be further improved by calibration of time offsets for individual pixels and time centroiding algorithms [54].

3.3 Afterpulsing

Afterpulsing is an important feature of the intensifier. It can be caused by secondary electrons or ions, which start another multiplication process in the vicinity of the primary pulse with a short delay [55]. The left part of Figure 5 illustrates these two afterpulsing mechanisms.

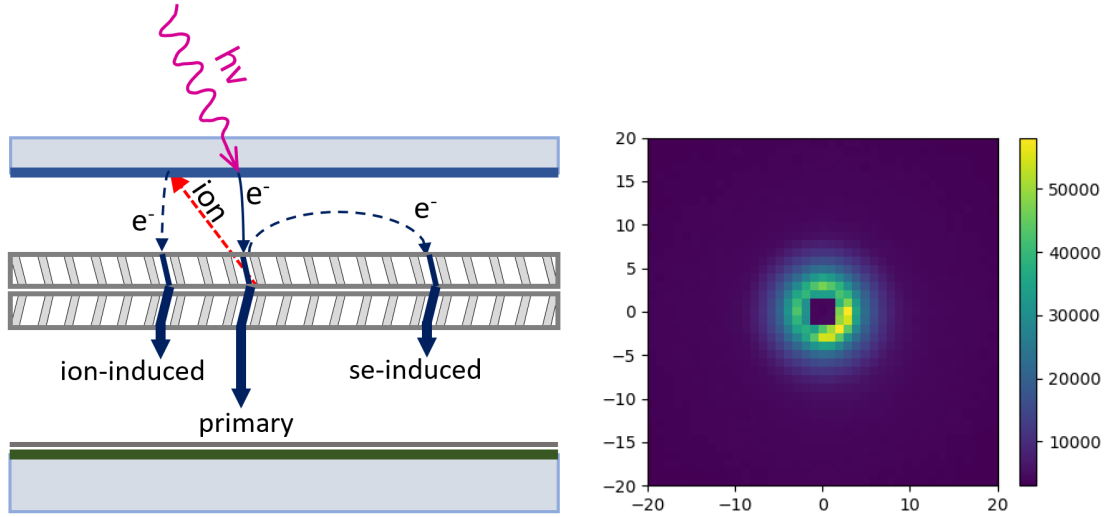


Figure 5. Left: Two mechanisms of afterpulsing due to the ion feedback and secondary electrons. Right: Spatial distribution of the afterpulses. The empty square 3×3 pixels in the middle is due to the requirement of the two hits to be separated by at least one pixel.

To find the afterpulses in the data, we look at the differences in time and position between the successive hits. The right part of Figure 5 shows a map of position differences in x and y for all consecutive in time pulses. There is an obvious excess of pulses spatially close to each other due to the afterpulsing. It also has an obvious asymmetry of the azimuthal distribution, which indicates a preferred direction, likely related to the orientation of the capillaries in the MCP glass. We verified this by rotating the intensifier by 90° with respect to the sensor, observing that the asymmetry followed the rotation.




Figure 6. Left: Distribution of distances for two successive hits. Right: Distribution of time differences for two successive hits.

To further characterize the afterpulsing, we plot the distributions of distance between the successive hits and their separation in time, see Figure 6. Note that the flat background in the time difference distribution is explained by random coincidences of dark count hits, with total rate of about 80 kHz. There is an obvious excess for the small values in both distributions, which we

estimate as deviations from the expected smooth behaviour and interpret as afterpulses. We found that the fraction of afterpulsing events closer than 10 pixels is 1.6% and fraction of afterpulsing events within 100 ns is 1.4%, which are satisfactorily close to each other values.

3.4 Bias voltage dependence




Figure 7. Normalized 2D occupancy for the intensifier dark counts for the silicon bias voltage between 0V and 60V.

Fully depleting silicon sensor is important for the camera operation with high detection efficiency. Figure 7 shows the normalized dark count images of an intensifier for the silicon bias voltage between 0V and 60V in Tpx3Cam. One can see that for low values of the bias voltage the silicon is not depleted showing characteristic stripes, so-called tree rings, due to variations of its resistivity [56, 57]. For the bias voltage above 30V, the structures are not visible, which agrees with expectations that the sensors are fully depleted at this voltage. A typical bias voltage used in the measurements is 50V.

4 Characterization of fast spectrometer based on the camera

Multiple quantum applications of the camera have been already mentioned in Section 2. Key to its successful employment was the efficient detection of multiple photons in the same device, which allowed a straightforward identification of their coincidences. Below we provide a detailed description of one of those experiments involving a single photon spectrometer.

Spectral binning of single photons for two-photon interferometry is a promising venue for various quantum applications [35, 58–61]. We implemented a simple dual spectrometer by sending two beams of collimated light on to a diffraction grating and then focusing them on to the intensified Tpx3Cam. The spectrometer was characterized using the argon spectrum, which has a large number of narrow lines. The resulting pattern is detected by the camera to produce an image like shown in the left part of Figure 8, with two horizontal stripes corresponding to two diffraction patterns produced by the same thermal argon source after splitting the beam in to two parts. In each of these stripes, distinct peaks can be seen, which can be interpreted as spectral lines of argon. The shown spectrum range is about 60 nm starting from 860 nm determined by the lens after the grating.

4.1 Linearity and spectral resolution

Since positions of the lines are well known we can use them for calibrations to determine the conversion scale and linearity. The right part of Figure 8 provides the scale and linearity graph with corresponding residuals.

Figure 9 shows three spectral lines: 794.8, 800.6 and 801.5 nm, for the same spectrometer with increased magnification. The lines are fitted with a Gaussian function with sigma 0.15 nm.




Figure 8. Left: Two argon spectra for two beams derived from the same argon lamp. Right: Spectrometer linearity, scale and residuals.




Figure 9. Left: Three argon lines in spectrometer with increased magnification. Right: Signal (top stripe) and idler (bottom stripe) photons in the spectrometer.

4.2 Spectral analysis of SPDC source

To demonstrate the performance of the spectrometer for single photons we used a Thorlabs SPDC source of photon pairs [62], where the signal and idler photons from the source were characterized in the two spectrometer channels. The full spectra of the photons are shown in the right part of Figure 9. The signal and idler photons in the pair anti-correlate in the wavelength to conserve the energy of pump photon. The left part of Figure 10 shows dependence of the signal wavelength on the idler wavelength for photon pairs within a 20 ns time window, where this anti-correlation is apparent. The right part of Figure 10 shows the reconstructed wavelength of the pump photon using the wavelengths of the signal and idler photons, and the argon spectrum calibration.

5 Conclusions

We described a fast optical camera with nanosecond scale timing resolution. The intensified version of the camera was successfully used in a variety of quantum applications, which required simultaneous detection and time stamping of multiple single photons.




Figure 10. Left: Anti-correlation of photon wavelengths for the SPDC source. Right: Reconstructed wavelength of the pump photon using the wavelengths of the signal and idler photons, and argon spectrum calibration.

Possible improvement to the described approach would be to switch to the next generation readout chip, Timepix4 [63], with timing resolution of 200 ps. The testing preparations are in progress though it remains to be seen if the optical path through the scintillator flashes registered by the silicon photodiode and Timepix4 front-end electronics would be fast enough to fully support the improved time resolution of Timepix4.

Acknowledgments

This work was supported by the U.S. Department of Energy QuantISED award and BNL LDRD grant 22-22. M.C., B.F. and R.M. acknowledge support under the Science Undergraduate Laboratory Internships (SULI) Program by the U.S. Department of Energy.

References

- [1] Giorgio Brida, Lucia Caspani, Alessandra Gatti, Marco Genovese, Alice Meda, and Ivano Ruo Berchera. Measurement of sub-shot-noise spatial correlations without background subtraction. *Phys. Rev. Lett.*, 102:213602, May 2009.
- [2] Matthew Reichert, Xiaohang Sun, and Jason W. Fleischer. Quality of spatial entanglement propagation. *Phys. Rev. A*, 95:063836, Jun 2017.
- [3] Bradley M. Jost, Alexander V. Sergienko, Ayman F. Abouraddy, Bahaa E. A. Saleh, and Malvin C. Teich. Spatial correlations of spontaneously down-converted photon pairs detected with a single-photon-sensitive ccd camera. *Opt. Express*, 3(2):81–88, Jul 1998.
- [4] Michał Jachura and Radosław Chrapkiewicz. Shot-by-shot imaging of hong–ou–mandel interference with an intensified sccm camera. *Opt. Lett.*, 40(7):1540–1543, Apr 2015.
- [5] Robert Fickler, Mario Krenn, Radek Lapkiewicz, Sven Ramelow, and Anton Zeilinger. Real-time imaging of quantum entanglement. *Scientific Reports*, 3:1914, May 2013.
- [6] Lijian Zhang, Leonardo Neves, Jeff S Lundeen, and Ian A Walmsley. A characterization of the single-photon sensitivity of an electron multiplying charge-coupled device. *Journal of Physics B: Atomic, Molecular and Optical Physics*, 42(11):114011, May 2009.

- [7] A. Avella, I. Ruo-Berchera, I. P. Degiovanni, G. Brida, and M. Genovese. Absolute calibration of an EMCCD camera by quantum correlation, linking photon counting to the analog regime. *Optics Letters*, 41(8):1841, Apr 2016.
- [8] Paul-Antoine Moreau, Ermes Toninelli, Thomas Gregory, and Miles J. Padgett. Imaging with quantum states of light. *Nature Reviews Physics*, 1(6):367–380, May 2019.
- [9] Leonardo Gasparini, Bänz Bessire, Manuel Unternährer, André Stefanov, Dmitri Boiko, Matteo Perenzoni, and David Stoppa. SUPERTWIN: towards 100kpixel CMOS quantum image sensors for quantum optics applications. In Manijeh Razeghi, editor, *Quantum Sensing and Nano Electronics and Photonics XIV*. SPIE, Jan 2017.
- [10] Matteo Perenzoni, Lucio Pancheri, and David Stoppa. Compact spad-based pixel architectures for time-resolved image sensors. *Sensors*, 16(5), 2016.
- [11] Myung-Jae Lee and Edoardo Charbon. Progress in single-photon avalanche diode image sensors in standard CMOS: From two-dimensional monolithic to three-dimensional-stacked technology. *Japanese Journal of Applied Physics*, 57(10):1002A3, Sep 2018.
- [12] Kazuhiro Morimoto, Andrei Ardelean, Ming-Lo Wu, Arin Can Ulku, Ivan Michel Antolovic, Claudio Bruschini, and Edoardo Charbon. Megapixel time-gated SPAD image sensor for 2d and 3d imaging applications. *Optica*, 7(4):346, Apr 2020.
- [13] Gur Lubin, Ron Tenne, Arin Can Ulku, Ivan Michel Antolovic, Samuel Burri, Sean Karg, Venkata Jayasurya Yallapragada, Claudio Bruschini, Edoardo Charbon, and Dan Oron. Heralded spectroscopy reveals exciton–exciton correlations in single colloidal quantum dots. *Nano Letters*, 21(16):6756–6763, August 2021.
- [14] Aleksander Divochiy, Francesco Marsili, David Bitauld, Alessandro Gaggero, Roberto Leoni, Francesco Mattioli, Alexander Korneev, Vitaliy Seleznev, Nataliya Kaurova, Olga Minaeva, Gregory Gol'tsman, Konstantinos G. Lagoudakis, Moushab Benkhaoul, Francis Lévy, and Andrea Fiore. Superconducting nanowire photon-number-resolving detector at telecommunication wavelengths. *Nature Photonics*, 2(5):302–306, Apr 2008.
- [15] Di Zhu, Marco Colangelo, Changchen Chen, Boris A. Korzh, Franco N. C. Wong, Matthew D. Shaw, and Karl K. Berggren. Resolving photon numbers using a superconducting nanowire with impedance-matching taper. *Nano Letters*, Apr 2020.
- [16] Boris Korzh, Qing-Yuan Zhao, Jason P. Allmaras, Simone Frasca, Travis M. Autry, Eric A. Bersin, Andrew D. Beyer, Ryan M. Briggs, Bruce Bumble, Marco Colangelo, Garrison M. Crouch, Andrew E. Dane, Thomas Gerrits, Adriana E. Lita, Francesco Marsili, Galan Moody, Cristián Peña, Edward Ramirez, Jake D. Rezac, Neil Sinclair, Martin J. Stevens, Angel E. Velasco, Varun B. Verma, Emma E. Wollman, Si Xie, Di Zhu, Paul D. Hale, Maria Spiropulu, Kevin L. Silverman, Richard P. Mirin, Sae Woo Nam, Alexander G. Kozorezov, Matthew D. Shaw, and Karl K. Berggren. Demonstration of sub-3 ps temporal resolution with a superconducting nanowire single-photon detector. *Nature Photonics*, 14(4):250–255, Mar 2020.
- [17] B. Cabrera, R. M. Clarke, P. Colling, A. J. Miller, S. Nam, and R. W. Romani. Detection of single infrared, optical, and ultraviolet photons using superconducting transition edge sensors. *Applied Physics Letters*, 73(6):735–737, Aug 1998.
- [18] Adriana E. Lita, Aaron J. Miller, and Sae Woo Nam. Counting near-infrared single-photons with 95% efficiency. *Optics Express*, 16(5):3032, 2008.
- [19] Robert H. Hadfield. Single-photon detectors for optical quantum information applications. *Nature Photonics*, 3(12):696–705, Dec 2009.

- [20] Peter Seitz and Albert JP Theuwissen, editors. *Single-Photon Imaging*. Springer Berlin Heidelberg, 2011.
- [21] Alan Migdall, Sergey V. Polyakov, Jingyun Fan, and Joshua C. Bienfang, editors. *Single-Photon Generation and Detection*, volume 45 of *Experimental Methods in the Physical Sciences*. Academic Press, 2013.
- [22] M. Fisher-Levine and A. Nomerotski. Timepixcam: a fast optical imager with time-stamping. *Journal of Instrumentation*, 11(03):C03016, 2016.
- [23] A. Zhao et al. Coincidence velocity map imaging using tpx3cam, a time stamping optical camera with 1.5 ns timing resolution. *Review of Scientific Instruments*, 88(9):113104, November 2017.
- [24] Andrei Nomerotski. Imaging and time stamping of photons with nanosecond resolution in timepix based optical cameras. *Nuclear Instruments and Methods in Physics Research Section A: Accelerators, Spectrometers, Detectors and Associated Equipment*, 937:26–30, September 2019.
- [25] www.amscins.com.
- [26] A. Nomerotski, I. Chakaberia, M. Fisher-Levine, Z. Janoska, P. Takacs, and T. Tsang. Characterization of timepixcam, a fast imager for the time-stamping of optical photons. *Journal of Instrumentation*, 12(01):C01017, 2017.
- [27] T. Poikela et al. Timepix3: a 65k channel hybrid pixel readout chip with simultaneous toa/tot and sparse readout. *Journal of instrumentation*, 9(05):C05013, 2014.
- [28] B. van der Heijden, J. Visser, M. van Beuzekom, H. Boterenbrood, S. Kulis, B. Munneke, and F. Schreuder. Spidr, a general-purpose readout system for pixel asics. *Journal of instrumentation*, 12(02):C02040, 2017.
- [29] <https://www.photonis.com/product/hi-qe-photocathodes>.
- [30] B. Winter, S. J. King, M. Brouard, and C. Vallance. A fast microchannel plate-scintillator detector for velocity map imaging and imaging mass spectrometry. *Review of Scientific Instruments*, 85(2):023306, February 2014.
- [31] D.A. Orlov, J. DeFazio, S. Duarte Pinto, R. Glazenberg, and E. Kernen. High quantum efficiency s-20 photocathodes in photon counting detectors. *Journal of Instrumentation*, 11(04):C04015–C04015, April 2016.
- [32] D.A. Orlov, T. Ruardij, S. Duarte Pinto, R. Glazenberg, and E. Kernen. High collection efficiency MCPs for photon counting detectors. *Journal of Instrumentation*, 13(01):C01047–C01047, jan 2018.
- [33] Christopher Ianzano, Peter Svihra, Mael Flament, Andrew Hardy, Guodong Cui, Andrei Nomerotski, and Eden Figueroa. Fast camera spatial characterization of photonic polarization entanglement. *Scientific Reports*, 10(1), Apr 2020.
- [34] Andrei Nomerotski, Dimitrios Katramatos, Paul Stankus, Peter Svihra, Guodong Cui, Sonali Gera, Mael Flament, and Eden Figueroa. Spatial and temporal characterization of polarization entanglement. *International Journal of Quantum Information*, 18(01):1941027, Feb 2020.
- [35] Yingwen Zhang, Duncan England, Andrei Nomerotski, Peter Svihra, Steven Ferrante, Paul Hockett, and Benjamin Sussman. Multidimensional quantum-enhanced target detection via spectrotemporal-correlation measurements. *Phys. Rev. A*, 101:053808, May 2020.
- [36] P. Svihra, Y. Zhang, P. Hockett, S. Ferrante, B. Sussman, D. England, and A. Nomerotski. Multivariate discrimination in quantum target detection. *arXiv:2005.00612*, May 2020.

- [37] A. Nomerotski, M. Keach, P. Stankus, P. Svihra, and S. Vintskevich. Counting of hong-ou-mandel bunched optical photons using a fast pixel camera. *arXiv:2005.07982*, May 2020.
- [38] Yingwen Zhang, Duncan England, Andrei Nomerotski, and Benjamin Sussman. High speed imaging of spectral-temporal correlations in hong-ou-mandel interference. *Optics Express*, 29(18):28217, August 2021.
- [39] Xiaoqin Gao, Yingwen Zhang, Alessio D’Errico, Khabat Heshami, and Ebrahim Karimi. High-speed imaging of spatiotemporal correlations in hong-ou-mandel interference. *Optics Express*, 30(11):19456, May 2022.
- [40] Yingwen Zhang, Antony Orth, Duncan England, and Benjamin Sussman. Ray tracing with quantum correlated photons to image a three-dimensional scene. *Physical Review A*, 105(1), January 2022.
- [41] Liudmila A. Zhukas, Peter Svihra, Andrei Nomerotski, and Boris B. Blinov. High-fidelity simultaneous detection of a trapped-ion qubit register. *Physical Review A*, 103(6), June 2021.
- [42] Liudmila A. Zhukas, Maverick J. Millican, Peter Svihra, Andrei Nomerotski, and Boris B. Blinov. Direct observation of ion micromotion in a linear paul trap. *Physical Review A*, 103(2), February 2021.
- [43] Alexander Kato, Apurva Goel, Raymond Lee, Zeyu Ye, Samip Karki, Jian Jun Liu, Andrei Nomerotski, and Boris B. Blinov. Two-tone doppler cooling of radial two-dimensional crystals in a radio-frequency ion trap. *Physical Review A*, 105(2), February 2022.
- [44] G. D’Amen, M. Keach, A. Nomerotski, P. Svihra, and A. Tricoli. Novel imaging technique for α -particles using a fast optical camera. *Journal of Instrumentation*, 16(02):P02006–P02006, February 2021.
- [45] A. S. Losko, Y. Han, B. Schillinger, A. Tartaglione, M. Morgano, M. Strobl, J. Long, A. S. Tremsin, and M. Schulz. New perspectives for neutron imaging through advanced event-mode data acquisition. *Scientific Reports*, 11(1), 2021.
- [46] Jianqing Yang, Jianrong Zhou, Xingfen Jiang, Jinhao Tan, Lianjun Zhang, Jianjin Zhou, Xiaojuan Zhou, Wenqin Yang, Yuanguang Xia, Jie Chen, XinLi Sun, Quanhu Zhang, Jiang Li, Zhijia Sun, and Yuanbo Chen. A novel energy resolved neutron imaging detector based on a time stamping optical camera for the CSNS. *Nuclear Instruments and Methods in Physics Research Section A: Accelerators, Spectrometers, Detectors and Associated Equipment*, 1000:165222, June 2021.
- [47] A. Roberts, P. Svihra, A. Al-Refaie, H. Graafsma, J. Küpper, K. Majumdar, K. Mavrokoridis, A. Nomerotski, D. Pennicard, B. Philippou, S. Trippel, C. Touramanis, and J. Vann. First demonstration of 3d optical readout of a TPC using a single photon sensitive timepix3 based camera. *Journal of Instrumentation*, 14(06):P06001–P06001, June 2019.
- [48] Liisa M. Hirvonen, Merlin Fisher-Levine, Klaus Suhling, and Andrei Nomerotski. Photon counting phosphorescence lifetime imaging with TimepixCam. *Review of Scientific Instruments*, 88(1):013104, January 2017.
- [49] Rajannya Sen, Liisa M. Hirvonen, Alexander Zhdanov, Peter Svihra, Stefan Andersson-Engels, Andrei Nomerotski, and Dmitri Papkovsky. New luminescence lifetime macro-imager based on a tpx3cam optical camera. *Biomed. Opt. Express*, 11(1):77–88, Jan 2020.
- [50] Rajannya Sen, Alexander V. Zhdanov, Thomaz F. S. Bastiaanssen, Liisa M. Hirvonen, Peter Svihra, Patrick Fitzgerald, John F. Cryan, Stefan Andersson-Engels, Andrei Nomerotski, and Dmitri B. Papkovsky. Mapping o₂ concentration in ex-vivo tissue samples on a fast PLIM macro-imager. *Scientific Reports*, 10(1), November 2020.

- [51] J Vallergera, A Tremsin, J DeFazio, T Michel, J Alozy, T Tick, and M Campbell. Optical mcp image tube with a quad timepix readout: initial performance characterization. *Journal of Instrumentation*, 9(05):C05055, 2014.
- [52] Arthur Zhao, Martin van Beuzekom, Bram Bouwens, Dmitry Byelov, Irakli Chakaberia, Chuan Cheng, Erik Maddox, Andrei Nomerotski, Peter Svihra, Jan Visser, Vaclav Vrba, and Thomas Weinacht. Coincidence velocity map imaging using tpx3cam, a time stamping optical camera with 1.5 ns timing resolution. *Review of Scientific Instruments*, 88(11):113104, November 2017.
- [53] S. Tsigaridas, M.v. Beuzekom, H.v.d. Graaf, F. Hartjes, K. Heijhoff, N.P. Hessey, P.J. de Jong, and V. Prodanovic. Timewalk correction for the timepix3 chip obtained with real particle data. *Nuclear Instruments and Methods in Physics Research Section A: Accelerators, Spectrometers, Detectors and Associated Equipment*, 930:185–190, June 2019.
- [54] K. Heijhoff, K. Akiba, R. Bates, M. van Beuzekom, P. Bosch, A.P. Colijn, R. Geertsema, V. Gromov, M.L.E. Heidotting, L.S. Hendrikx, D. Hynds, and H. Snoek. Timing measurements with a 3d silicon sensor on timepix3 in a 180 GeV/c hadron beam. *Journal of Instrumentation*, 16(08):P08009, August 2021.
- [55] D. A. Orlov, R. Glazenberg, R. Ortega, and E. Kernén. Uv/visible high-sensitivity mcp-pmt single-photon ghz counting detector for long-range lidar instrumentations. *CEAS Space Journal*, 11(4):405–411, Dec 2019.
- [56] S E Holland, C J Bebek, W F Kolbe, and J S Lee. Physics of fully depleted CCDs. *Journal of Instrumentation*, 9(03):C03057–C03057, March 2014.
- [57] H.Y. Park, A. Nomerotski, and D. Tsybychev. Properties of tree rings in LSST sensors. *Journal of Instrumentation*, 12(05):C05015–C05015, May 2017.
- [58] E. T. Khabiboulline, J. Borregaard, K. De Greve, and M. D. Lukin. Optical interferometry with quantum networks. *Phys. Rev. Lett.*, 123:070504, Aug 2019.
- [59] P. Stankus, A. Nomerotski, A. Složar, and S. Vintskevitch. Two-photon amplitude interferometry for precision astrometry. *arXiv preprint arXiv:2010.09100*, 2020.
- [60] A. Nomerotski, P. Stankus, A. Složar, S. Vintskevich, S. Andrews, G. A. Carini, D. Dolzhenko, D. England, E. V. Figueroa, S. Gera, J. Haupt, S. Herrmann, D. Katramatos, M. Keach, A. Parsells, O. Saira, J. Schiff, P. Svihra, T. Tsang, and Y. Zhang. Quantum-assisted optical interferometers: instrument requirements. In Antoine Mérand, Stephanie Sallum, and Peter G. Tuthill, editors, *Optical and Infrared Interferometry and Imaging VII*, Proc. SPIE, 2020.
- [61] Matthew Brown, Valerian Thiel, Markus Allgaier, Michael Raymer, Brian Smith, Paul Kwiat, and John Monnier. Long-baseline interferometry using single photon states as a non-local oscillator. In Philip R. Hemmer and Alan L. Migdall, editors, *Quantum Computing, Communication, and Simulation II*. SPIE, March 2022.
- [62] Thorlabs. *SPDC810 Correlated Photon-Pair Source*.
- [63] X. Llopart, J. Alozy, R. Ballabriga, M. Campbell, R. Casanova, V. Gromov, E.H.M. Heijne, T. Poikela, E. Santin, V. Sriskaran, L. Tlustos, and A. Vitkovskiy. Timepix4, a large area pixel detector readout chip which can be tiled on 4 sides providing sub-200 ps timestamp binning. *Journal of Instrumentation*, 17(01):C01044, January 2022.