

EQUIPMENT FOR SS 90

(3S90-000-3)

A SPECIFICATION

The provisional equipment of ss 90 is a horizontal dipole (4C02-100-3) and a standard elliptic vacuum chamber (3A65-703-4) - (P. Riboni, F. Rohner).

1. The requirements for precision and stability of alignment of the elements are :

$$\left\{ \begin{array}{l} \pm 1 \text{ mm radially,} \\ \pm 0,5 \text{ mm vertically,} \\ \pm 1 \text{ mrad in angle perpendicular to the beam.} \end{array} \right.$$

It follows that the precision of the initial installation, because of the rigidity of the supporting structure, is only a fraction of the given values.

2. The horizontal dipole is a split magnet, which allows the mounting of the element in the PS ring, independently of the vacuum chamber.

3. The provisional vacuum chamber is of standard type, with standard two-point quick-couplings both sides.

4. The dipole and the vacuum chamber are sitting on the main support, each having its individual alignment system.

5. The main support is aligned in height to $\pm 0,2$ mm by means of shims. The elements are adjusted in the laboratory to the required height. The angular and radial movements are done in the ring.

6. The vacuum chamber is built on the support and aligned. Then the split dipole is assembled in situ, with the electric and water connections towards the inside of the ring (F. Rohner), and adjusted.

B ALIGNMENT AND ASSEMBLY PROCEDURE

a) Work in the laboratory and workshop

1. Assembly of the horizontal dipole on its individual support mechanism.
Alignment in horizontal plane with shims : $\pm 0,2$ mm.
2. Welding of vacuum chamber.
3. Vacuumtest of chamber.

b) Work in the PS ring

1. Installation and alignment of the main support by means of shims. The reference-faces are the two rails on top of the bedplate.

Alignment in horizontal plane : $\pm 0,2$ mm with spirit level and for the absolute height the surveyors.

Radial positionning : ± 2 mm with the jig (3T04-000-S4)


Drawing : 4C02-600-3.

2. Mounting of the vacuum chamber on the main support.
3. Mounting of the dipole on the main support.
4. Alignment of the elements in radial sense with jig (4T-002-2).

ANNEX : 3590-000-3.

Distribution

E. Boltezar
L. Henny
U. Jacob
P.H. Mann
G. Plass
P. Riboni
F. Rohner
C.E. Rufer

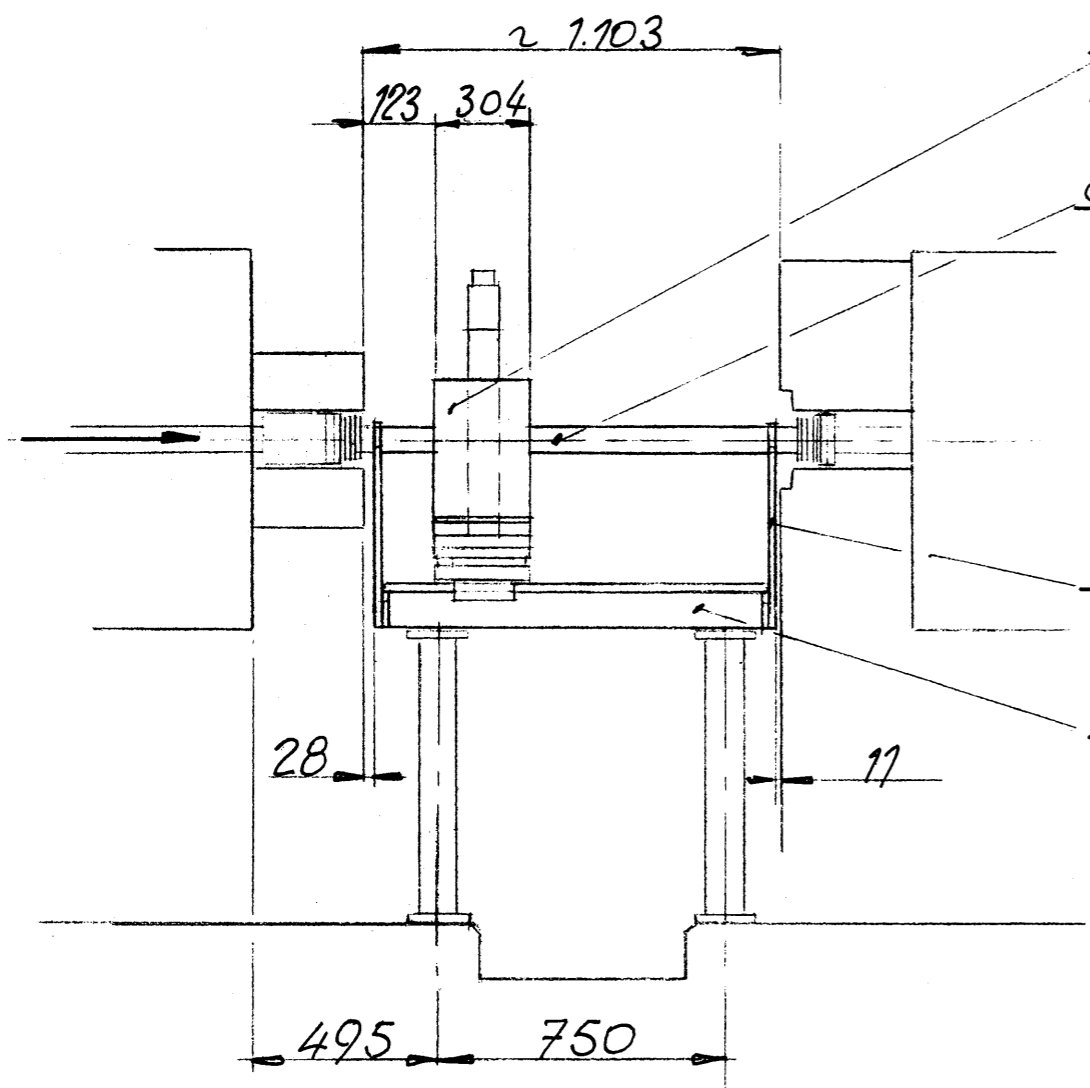


Dipole horiz.
4C02.100.3


chambre à vide
3A65.703.4

Support
4C02.500.4

Support princ.
4C02.600.3

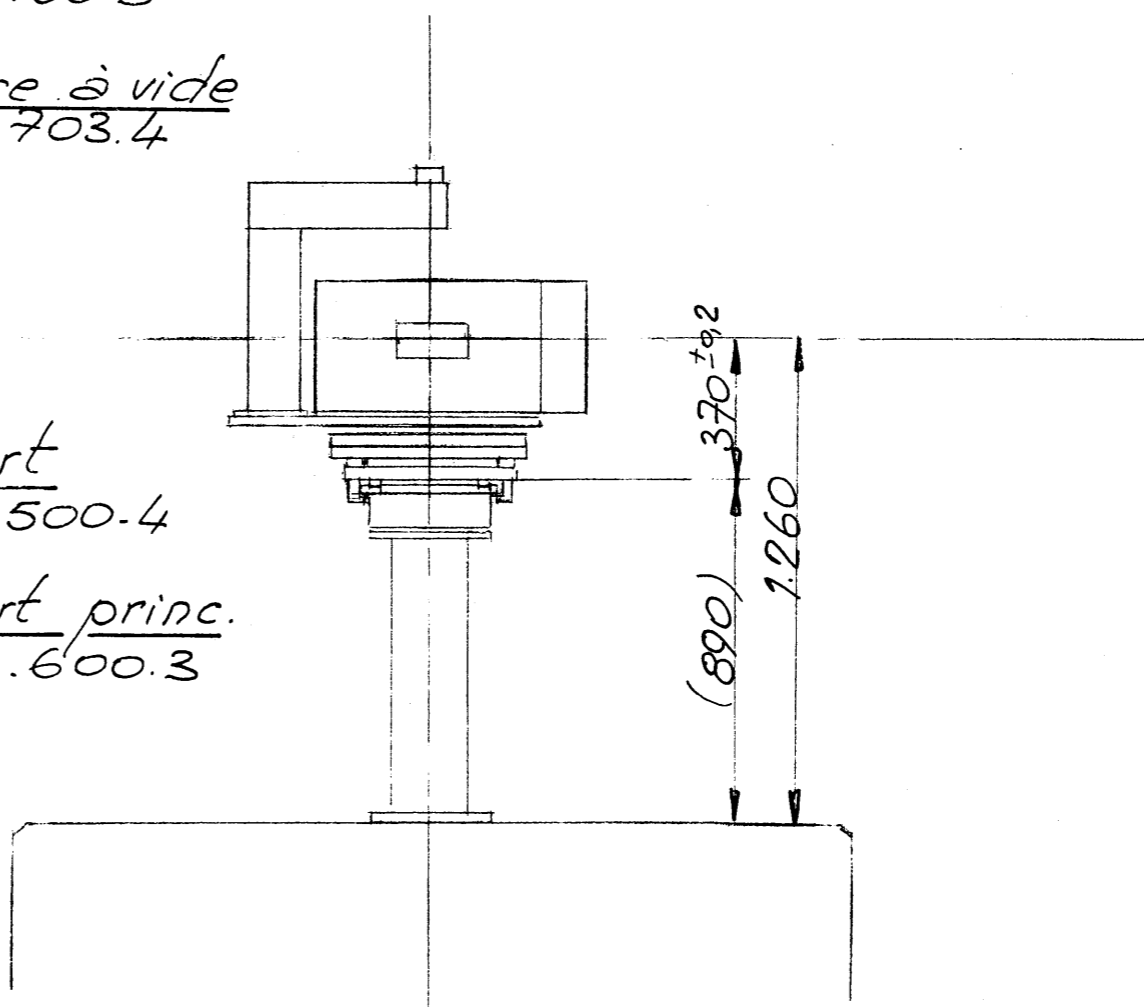

Gabarit d'alignement: pour dip horiz: 4T.002.2

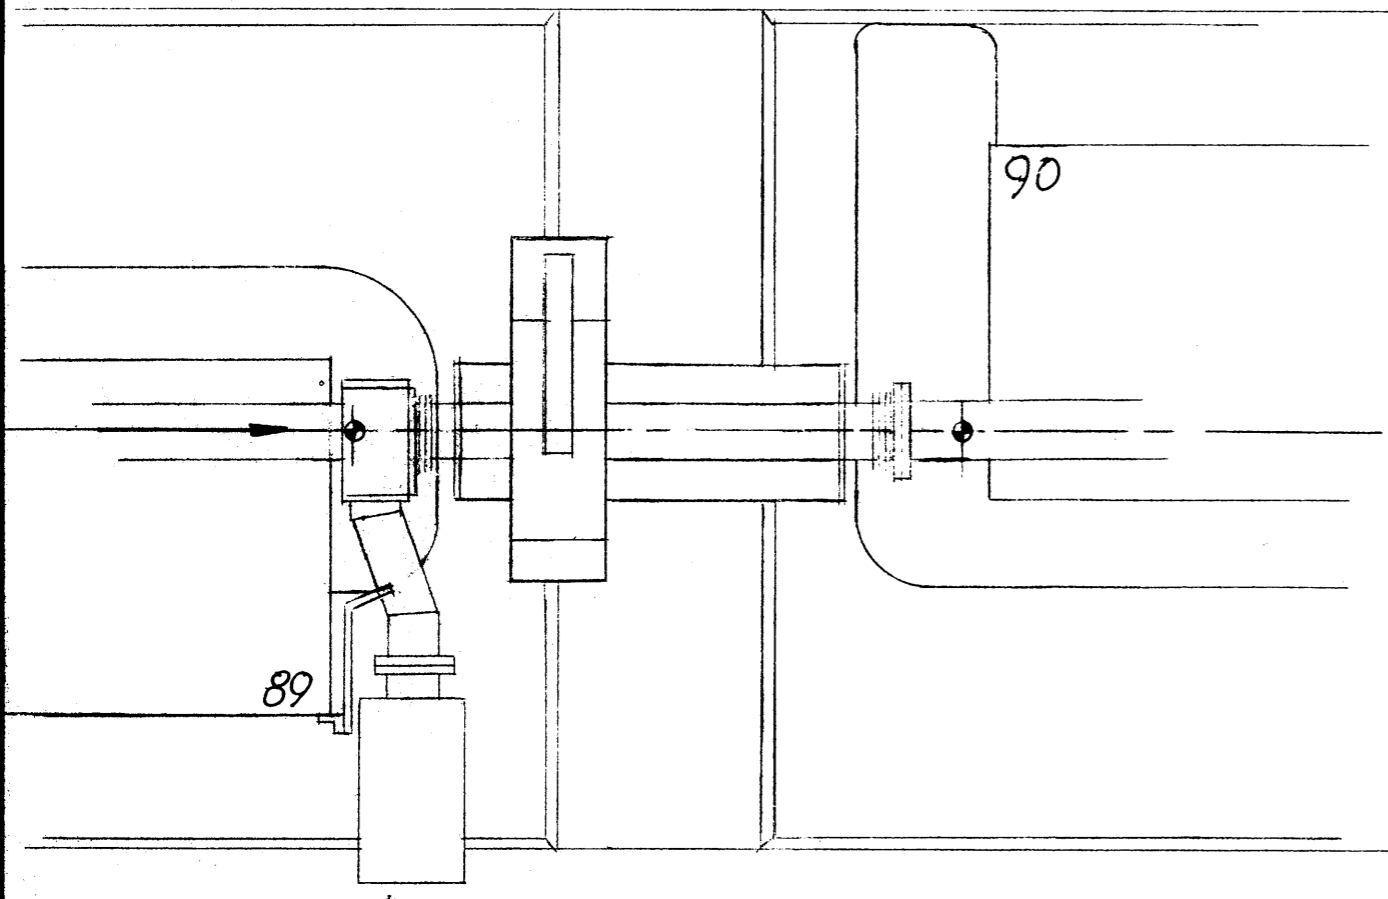

NOMBRE DE PIÈCES	DÉSIGNATION	POS.	MATIÈRE	OBSERVATIONS	
		Section droite 90			ECHELLE
	Dipole horizontal				CONTROLÉ 1.72 R.S.
				1/20	VU
					REMPLECE
					REMPLECE PAR
					RÉDUCTION

CERN ORGANISATION EUROPÉENNE POUR
LA RECHERCHE NUCLÉAIRE - GENÈVE

M.P.S.3590.000.3