

Measurements and Simulations of Ionization Chamber Signals in Mixed Radiation Fields for the LHC BLM System

B. Dehning, Ch. Fabjan, G. Ferioli, E.B. Holzer, M. Stockner.

CERN – Geneva - Switzerland

Abstract

The LHC beam loss monitoring (BLM) system must prevent the super conducting magnets from quenching and protect the machine components from damage. The main monitor type is an ionization chamber. About 4000 of them will be installed around the ring. The lost beam particles initiate hadronic showers through the magnets, which are measured by the monitors installed outside of the cryostat around each quadrupole magnet. They probe the far transverse tail of the hadronic shower. The specification for the BLM system includes a factor of two absolute precision on the prediction of the quench levels. To reach this accuracy a number of simulations are being combined to calibrate the monitor signals. To validate the monitor calibration the simulations are compared with test measurements. This paper will focus on the simulated prediction of the development of the hadronic shower tails and the signal response of ionization chambers to various particle types and energies. Test measurements have been performed at CERN and DESY and compared to Geant4 simulations.

Presented at IEEE 2006 – 29th Oct – 4th Nov 2006 –San Diego/CA - USA

Measurements and Simulations of Ionization Chamber Signals in Mixed Radiation Fields for the LHC BLM System

Markus Stockner, Bernd Dehning, Christian Fabjan, Gianfranco Ferioli, and Eva Barbara Holzer

Abstract—The LHC beam loss monitoring (BLM) system must prevent the superconducting magnets from quenching and protect the machine components from damage. The main monitor type is an ionization chamber. About 4000 of them will be installed around the ring. The lost beam particles initiate hadronic showers through the magnets, which are measured by the monitors installed outside of the cryostat around each quadrupole magnet. They probe the far transverse tail of the hadronic shower. The specification for the BLM system includes a factor of two absolute precision on the prediction of the quench levels. To reach this accuracy a number of simulations are being combined to calibrate the monitor signals. To validate the monitor calibration the simulations are compared with test measurements. This paper will focus on the simulated prediction of the development of the hadronic shower tails and the signal response of ionization chambers to various particle types and energies. Test measurements have been performed at CERN and DESY and compared to Geant4 simulations.

Index Terms—LHC BLM, beam loss monitoring, Geant4.

I. INTRODUCTION

THE LHC is a proton collider with injection energy of 450 GeV and top energy of 7 TeV. Two counter rotating beams are crossing each other at the interaction points (IP). The stored energy is 360 MJ maximum per beam (enough to melt 500 kg of copper) and 10 GJ in the magnet system [1]. Lost beam protons can quench the magnets or even destroy machine components. There are several safety systems to protect the machines components from damage. One of them is the Beam Loss Monitoring (BLM) system that measures the lost beam protons outside of the magnet cryostats [2]. The main detector type is an ionization chamber. About 4000 will be installed. At special locations (e.g. collimator regions) additional secondary emission monitors (SEM) are used to increase the dynamic range from 10^8 to 10^{13} . The detectors probe the transverse tails of the hadronic showers through the cryostats which are induced by lost beam particles.

The start-up calibration of the BLM system is designed to be within a factor of five in accuracy and for the final calibration a factor of two is required. A number of simulations were performed to calibrate the system. The beam particles were tracked to find the most probable loss locations. At these loss locations hadronic showers through the machine components

Manuscript received November 17, 2006.

M. Stockner is with CERN and Vienna University of Technology. All authors are with CERN, CH-1211 Geneva 23, Switzerland (e-mail: firstname.lastname@cern.ch).



Fig. 1. LHC beam loss monitors (yellow insulation) mounted on a red support outside on a cryostat. They are horizontally aligned to the beam pipe.

are simulated to get the particle spectra at the detector locations. The spectra will be further used to simulate the detector signal. The quench levels of the superconducting magnets, according to loss duration and beam energy, are simulated separately. This paper will focus on the detector response simulation, which is part of the system calibration and on the uncertainty estimation of transverse hadronic shower tail simulations, which is part of the system calibration error. The simulations are verified by measurements performed at CERN and DESY.

II. IONIZATION CHAMBER RESPONSE SIMULATION

Signal speed and robustness against aging were the main design criteria for the detectors.



Fig. 2. Inside structure of the LHC BLM (ionization chamber).

Because of the high dynamic range an ionization chamber and a secondary emission monitor will be used.

This paper will focus on the ionization chambers with parallel aluminum electrode plates separated by 0.5 cm, as shown in Fig. 2. The detectors are about 50 cm long with a diameter of 9 cm and a sensitive volume of 1.5 liter. The collection time of the electrons and ions is of the order of 300 ns and 80 μ s respectively. The chambers are filled with N_2 at 100 mbar overpressure [2].

Depending on the loss location the detectors will be exposed to different radiation fields. The energy of the particles is spread over a large range from keV to TeV and their number is exponentially decreasing with energy.

Geant4 (version 8.0 patch-01) [3] simulations of the ionization chambers were performed to determine the signal response for different particle types at various kinetic energies in the range of 10 keV to 10 TeV. Longitudinal (Fig. 3) and transverse (Fig. 4) impacting directions in respect to the detector axis were simulated. The longer path for a longitudinal direction increased the response approximately by a factor of two. Less wall material has to be passed for the transverse direction, that leads to a lower energy cut-off. The deposited energy in the sensitive volume was converted with the so called W-value to the number of produced charges. The W-value for N_2 is 35 eV per electron-ion pair [4].

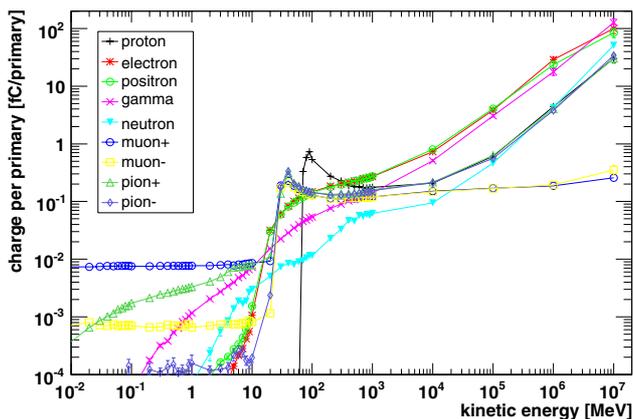


Fig. 3. Response of the ionization chamber for particles impacting longitudinally to the detector axis.

The following parameters in the simulation were varied to identify different contributions to the systematic error. The impacting angle causes a variation of the detector response; at high energy up to a factor of 100 for protons. The standard production range cut (1 mm) in Geant4 was changed to 10 μ m (one fiftieth of the electrode thickness). This increased the detector response by 12%. A further decrease to smaller values (1 nm) would increase the results additionally by 3%, but increases the CPU time further.

The sensitive volume was determined by simulation of the electric field configuration. It is 4% bigger than the volume covered by the electrodes (2 mm larger diameter). NIST data were used to cross check the simulation [5]: The energy cut-off for protons, electrons and gamma rays was estimated. Protons

of about 65 MeV start to produce a signal, electrons at 9 MeV and gammas at 150 keV (parallel impact to detector axis).

The energy deposition for a positive muon was calculated with the Bethe-Bloch formula and compared to the simulation (agreement at 1 GeV: 95% and at 35 MeV: 75%).

The strong rise in the detector response for high kinetic energies, in case of longitudinal impact (Fig. 3), was investigated. Depending on the relative impacting point of the particles to the inner structure more or less dense material has to be crossed. In denser material a larger number of interactions occur and the relative signal rises (e.g. stainless steel rods holding the electrodes).

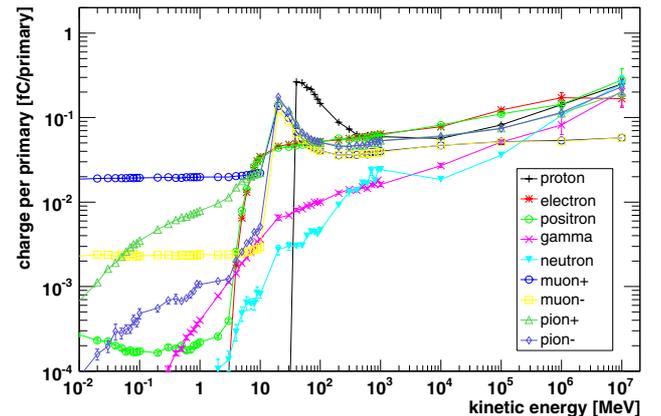


Fig. 4. Response of the ionization chamber for particles impacting transversely to the detector axis.

III. VERIFICATION MEASUREMENTS

Three measurements with different particle types and energies were performed to validate the Geant4 simulations.

A. Mixed Radiation Field Measurement

A mixed radiation field experiment at the CERF target area (CERN-EU High Energy Reference Field Facility) was compared to the simulation. A copper target (length 50 cm, diameter 7 cm) was placed in a secondary beam of 120 GeV/c hadrons. The main beam particles were pions (60.7%), protons (34.8%) and kaons (4.5%) with intensities up to $9.5 \cdot 10^7$ hadrons per 4.8 seconds. Five ionization chambers were positioned around the copper target so that they are exposed to different radiation fields (varying in particle composition and energy).

The CERF team had performed a similar experiment with PMI (air filled plastic ionization chamber) detectors and verified it by FLUKA simulations [6]. Their FLUKA spectra were used as input to simulate the detector response with Geant4. A comparison of the Geant4 simulation to the BLM detector measurement shows a relative difference of about 12%, except at detector position 1 (Table I). There, a relative difference of 21% can be seen. The detector specific energy cut-off and the shift of the particle spectrum to lower energies (below

TABLE I
RESULT OF GEANT4 SIMULATIONS, BEAM MEASUREMENTS AND
THEIR COMPARISON AT THE CERF TARGET AREA
(10^{-12} COULOMB PER $9.2 \cdot 10^7$ HADRONS).

pos.	Geant4 sim. [pC]		measurement [pC]		ratio	
	SPS BLM	error	SPS BLM	error	sim/meas.	error
1	91.13	0.35	115.33	11.66	0.79	0.08
2	281.22	5.98	—	—	—	—
3	1656.38	18.21	1577.75	162.59	1.05	0.11
4	2386.62	21.53	2121.52	230.69	1.12	0.12
5	3943.99	23.12	3531.98	370.42	1.12	0.12
6	6495.5	17.54	7091.16	1096.82	0.92	0.14

1 GeV) leads to a low statistics in the number of particles that contribute to the detector signal. A comparison of the spectra between position 1 and position 6 is shown in Fig. 5. The error on the measurement includes the statistical error, a systematic error from uncertainties on the beam intensity measurement (10%) and from misalignment investigations on the detector positions [6]. The error on the simulation includes only the statistical error of the signal simulation, it does not include the uncertainties in the spectrum.

All detectors showed a linear behavior at measurements over one order of magnitude in beam intensity (up to $9.5 \cdot 10^7$ hadrons onto the copper target). A first order polynomial fit showed for the detectors 3 to 6 a χ^2/ndf between 5/5 and 10/5, and for detector 1 a χ^2/ndf of 36/5.

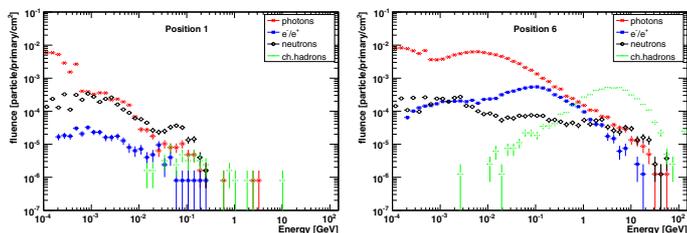


Fig. 5. FLUKA spectra for up- and down-stream position at the CERF target area [6].

B. 400 GeV/c Proton Measurement

A second experiment with 400 GeV/c protons at an SPS extraction line (T2) was compared to the simulation. The beam size was estimated to 1 cm horizontally and 0.5 cm vertically (4σ). The intensity was $30.0 \cdot 10^{11} \pm 0.1 \cdot 10^{11}$ protons per 4.8 seconds. With Geant4 a vertical scan of the beam position in the simulation was compared to the measurement. The unknown beam position (vertically) relative to the inner structure (parallel electrodes) led to a systematic uncertainty of 23%. Measurement and simulation agree within errors (Table II).

C. Gamma Ray Measurement

A third comparison between simulation and measurement was done for gamma rays at the TIS-RP Calibration Laboratory

TABLE II
400 GeV/c PROTON MEASUREMENT RESULTS
(CHARGES PER PROTON PER CM).

simulation [q/(p-cm)]		measurement [q/(p-cm)]		ratio	
BLM	sys. error	BLM	error	sim./meas.	error
124.84	25	110	0.06	1.13	0.23

for Radiation Protection Instruments (CERN). The measurement was done with Cs137 sources at various activities and distances. The detector showed once more a linear behavior within two orders of magnitude in dose rate ($3 \mu\text{Sv/h}$ to 3mSv/h). The response simulation results for 600 keV and 700 keV gamma rays were interpolated and compared to the measurement results. The measurement and the simulation agree within 64% with an error of 7% (Table III).

TABLE III
GAMMA RAY MEASUREMENT RESULTS (10^{-18} COULOMB PER PHOTON).

simulation [aC/ γ]		measurement [aC/ γ]		ratio	
BLM	error	BLM	error	sim./meas.	error
0.27	0.02	0.42	0.01	0.64	0.05

D. Neutron Measurement

Further verification and calibration measurements are planned for November 2006 at the Svedberg Laboratory, Uppsala University (Sweden) [7].

IV. HADRONIC SHOWER MEASUREMENTS AT HERA

The LHC BLM system start-up calibration is based on Geant3 and Geant4 simulations. Hadronic showers through LHC components and the detector response were simulated. An experiment at the HERA proton beam dump was set up to estimate the error on the far transverse hadronic shower tail simulations with Geant4. Six ionization chambers were installed on top of the dump, with a longitudinal spacing of about 1 m. At this parasitic experiment the far transverse tails of hadronic showers can be measured. The impacting protons have energies of 40 GeV (injection) and 920 GeV (top energy). The intensity is in the range of $1.3 \cdot 10^{11}$ to $1.3 \cdot 10^{13}$ protons. The estimated error on the transverse hadronic shower tail simulations will be part of the BLM system calibration error. The simulation was split into two parts. First, the primary proton beam onto the dump was simulated and all particles arriving at the top of the dump were scored. In the second part, these secondary particles were launched for each detector position to get the detector signal. Two vertically separated impacting points on the dump were chosen to simulate the sweeping of the protons. The simulations were performed with Geant4 8.0 (patch-01) and the QGSP physics list. The LHC BLM electronics was used to measure the detector signal. It consists of a CFC (current to frequency converter) and an FPGA (field

programmable gate array) board, which provides the signal integrated over time windows, ranging from $40 \mu\text{s}$ to 80s [8]. The short particle pulse (one HERA turn corresponds to $21 \mu\text{s}$) hitting the ionization chamber creates a high current (up to 1 A). A large filter ($\tau = R \cdot C = 170 \text{ms}$) had to be installed in the input chain as the maximum input current to the electronic is 1 mA.

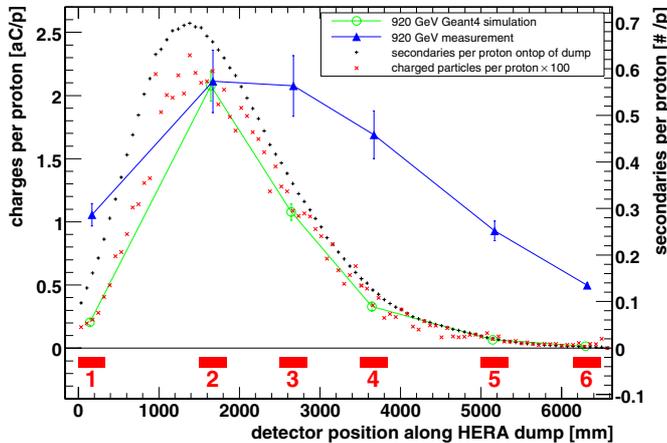


Fig. 6. Detector signal from simulation and measurement versus detector position on the HERA proton beam dump (preliminary data). Detector positions (in scale) at the bottom of the plot.

The simulation and measurement is in good agreement close to the shower maximum (detector position 2 in Fig. 6). The disagreement for the other detectors is not yet understood. It can be seen from Fig. 6 that uncharged particles dominate the spectra (less than 1% charged particles). Further investigations with different physics lists are planned, e.g. QGSP_BERT_HP (bertini models, high precision neutron transport) or QGSP_BIC_HP (binary cascade, high precision neutron transport), to identify possible systematic errors. Simplifications in the simulation were made: The beam size, the impacting angle ($\approx 1.5 \text{mrad}$) and the tunnel geometry were not taken into account. These may also lead to greater uncertainties. The calibration of the readout electronic as function of input current led to a correction of maximal 20%. A final electronics calibration has to be done. Recombination effects due to the short high intensity pulses will also be subject of further investigations.

V. CONCLUSION

The Geant4 detector response simulations are part of the LHC BLM calibration. The simulations were successfully performed and verified by different measurements. At the CERF target area the detector response in a mixed radiation field was compared to Geant4 simulations. The agreement is within the error, except for the upstream detector. At this position the detector specific energy cut-off and the shift of the particle spectrum to lower energies leads to a low statistics in the number of particles that contribute to the detector signal. The comparison of an experiment in a $400 \text{GeV}/c$ proton beam is in

agreement with the simulation. A comparison of a gamma ray measurement (Cs137) with the simulated detector response was within 36%. An experiment at the HERA proton beam dump to estimate the error of Geant4 far transverse hadronic shower tail simulations was performed. The comparison of measurement and simulation close to the shower maximum shows a good agreement. At the other positions the simulation differs from the measurement. Over a period of 6 months the LHC BLM electronics was successfully used for this experiment. Further verification tests at the Svedberg Laboratory, Uppsala University (Sweden) [7] are planned for November 2006.

ACKNOWLEDGMENT

The authors would like to acknowledge the contributions of various members of the LHC BLM section [9].

REFERENCES

- [1] R. Schmidt et al., *Protection of the CERN large hadron collider*, New Journal of Physics, accepted for publication, 2006.
- [2] E. B. Holzer et al., *Beam Loss Monitoring System for the LHC*, IEEE NSS-MIC '05, Puerto Rico, CERN-AB-2006-009 BI, 2005.
- [3] Geant4 collaboration, *Geant4 Simulation Toolkit*, <http://geant4.web.cern.ch/geant4>, viewed October 30, 2006.
- [4] International Commission on Radiation Units and Measurements, *Average Energy Required To Produce An Ion Pair*, ICRU Report 31, Washington D.C., (1979).
- [5] NIST (National Institute of Standard and Technology) Standard Reference Database 124, *Stopping-Power and Range Tables for Electrons, Protons, and Helium Ions*, <http://physics.nist.gov/PhysRefData/Star/Text/contents.html>, viewed March 3, 2006.
- [6] H. Vincke, N. Aguilar, D. Forkel-Wirth, M. Pangallo, D. Perin, M. Renou, C. Theis, *Measurements and Simulations of the PMI Chamber Response to the Radiation Field inside the CERF Target Area*, CERN EDMS No.: 457013, (CERN-SC-2004-025-RP-TN).
- [7] A. V. Prokofiev, O. Byström, C. Ekström, V. Ziemann, J. Blomgren, S. Pomp, M. Oesterlund, and U. Tippawan, *A New Neutron Beam Facility at TSL*, International Workshop on Fast Neutron Detectors and Applications, University of Cape Town, South Africa, (FNDA2006 016), 2006.
- [8] W. Friesenbichler, *Development of the Readout Electronics for the Beam Loss Monitors of the LHC*, CERN-THESIS-2002-028, Diplomarbeit, Fachhochschule W. Neustadt, 2002.
- [9] C. Zamantzas et al., *The LHC beam loss monitoring system's real-time data analysis card*, CERN-AB-2005-082, DIPAC 05, Lyon, France, 2005.
- [10] C. Zamantzas, *The Design, Construction, Test and Integration of the LHC Beam Loss Monitor Threshold Comparator (BLMTC)*, PhD Thesis, Brunel University, London, UK, 2006.
- [11] C. Zamantzas, B. Dehning, E. Effinger, J. Emery, G. Ferioli, *An FPGA Based Implementation for Real-Time Processing of the LHC Beam Loss Monitoring System's Data*, IEEE NSS-MIC '06, San Diego, IEEE Trans. Nucl. Sci., submitted for publication, 2006.
- [12] www.cern.ch/blm