# Comparison of High Energy X-Ray and Cobalt-60 Irradiations on MOS Capacitors

Vincent Girones<sup>®</sup>, Jérôme Boch<sup>®</sup>, Frédéric Saigné, Alain Carapelle<sup>®</sup>, *Member, IEEE*, Arnaud Chapon, Tadec Maraine, and Rubén García Alía<sup>®</sup>, *Member, IEEE* 

Abstract—The use of a high energy X-ray generator for Total Ionizing Dose (TID) testing is studied on metal-oxide semiconductor (MOS) capacitors. Several conditions were studied for the high energy X-ray irradiations (with aluminum and lead filters) and the experimental results are compared to Cobalt 60 (Co-60) irradiations. The effects of both annealing and package lid are also studied. All of the results are presented and discussed. It is shown that the simple BEOL stack (only one thin aluminum layer) has no effect on dose deposition in the oxide of MOS capacitors.

Index Terms—Cobalt-60, dose testing, high energy X-ray, metal-oxide semiconductor (MOS) capacitor, total ionizing dose (TID).

#### I. Introduction

VER the past decade, efforts have been made to reduce the world's dependence on high-level radioactive sources, particularly Cobalt 60 (Co-60) and Cesium 137 [1], [2], [3]. These sources are used in commercial, medical, and research applications throughout the world. The main objective, as a security strategy, is to replace high-risk radioactive sources with less risky alternatives in order to enhance radiological security and to forestall an act of radiological terrorism. In the field of reliability of electronic components and systems, for space, military, accelerator, and nuclear power plants applications, such radioactive sources are used for Total Ionizing Dose (TID) testing. These sources are used because they are recommended by current testing standards such as MIL-STD-883 test method (TM) 1019 for TID qualification and Radiation Lot Acceptance Testing (RLAT) [4], ESA ESCC Basic Specification No. 22900 [5], and ASTM F 1892 Standard Guide for Ionizing Radiation (Total Dose) Effects Testing of Semiconductor Devices [6]. These standards specify electronic devices testing using irradiation from

Manuscript received 27 December 2023; revised 31 January 2024; accepted 8 February 2024. Date of publication 23 February 2024; date of current version 16 August 2024. This work was supported by the European Union Project RADNEXT through the European Union's Horizon 2020 Research and Innovation Program under Agreement 101008126. (Corresponding author: Vincent Girones.)

Vincent Girones, Jérôme Boch, Frédéric Saigné, and Tadec Maraine are with the UM, UMR UM/CNRS 5214, Université de Montpellier, F-34095 Montpellier, France (e-mail: vincent.girones@umontpellier.fr).

Alain Carapelle is with the Centre Spatial de Liège (CSL), 4031 Angleur, Belgium.

Arnaud Chapon is with ATRON Metrology, 50130 Cherbourg-en-Cotentin, France.

Rubén García Alía is with the European Organization for Nuclear Research (CERN), CH-1211 Geneva, Switzerland.

Color versions of one or more figures in this article are available at https://doi.org/10.1109/TNS.2024.3366432.

Digital Object Identifier 10.1109/TNS.2024.3366432

photons sources, such as Co-60  $\gamma$  irradiators, Cesium 137  $\gamma$  irradiators, electron beams, and low energy (approximately 10 keV) X-ray generators. However, Co-60 remains the most common radiation source used for TID testing of electronic components and systems. Co-60 is usually considered as the reference ionizing radiation source to perform TID tests on electronic devices and systems. In order to meet the above requirements in terms of security, alternative solutions must be found.

The use of a high-energy X-ray generator has recently been proposed to perform TID testing [7]. In the context of electronics, and in accordance with the above-mentioned standards, generators of over 100 kV are considered to be high-energy X-ray generators. Photons of 100 keV interact in a Compton predominant effect for the majority of elements making up electronic systems. X-ray generators are generally considered much more convenient for TID testing and offer many advantages: 1) safety and security issues are more easily managed with an X-ray generator than with radioactive sources; 2) the photon energies are low enough that it can be easily collimated that allows irradiating a single part on a board; 3) X-ray generator offers a relatively high dose rate, thus offering reduced testing time; and 4) X-ray generators are less expensive to purchase and maintain than radioactive sources. Moreover, high-energy X-ray generators offer the possibility to test packaged devices due to high penetration depths.

In [7], a high-energy X-ray generator was used with a lead filter in order to attenuate low-energy photons of the energy spectrum, i.e., reduce the photoelectric effect and get closer to Compton scattering processes. It has been shown (on metal–oxide semiconductor (MOS) and bipolar transistors) that, with such a lead filter, it is possible to approach the degradation obtained with a Co-60 irradiation and this is all the more true as the voltage of the tube (the maximum energy of the photons) is high. However, a gap in the observed degradation between high-energy X-rays with a lead filter and Co-60 irradiations remains. This gap has been attributed to packaging or backscattered photons in Back-End-of-the-Line (BEOL) stack (contacts, metal layers, insulating layers) that can have a significant TID contribution in the sensitive oxide of the investigated devices [8]. This stack of layers can also induce dose enhancement, which is a function of the photon energy (with a higher dose enhancement factor for low energy photons) and is larger for high Z elements [9], [10], [11], [12], [13], [14], [15], [16], [17], [18], [19].

Since dose enhancement occurs mainly with low-energy photons and metallization with high Z values, as shown in

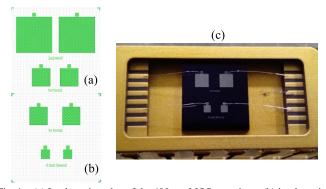


Fig. 1. (a) Implantation plan of the 400 nm MOS capacitors, (b) implantation plan of the 100 nm MOS capacitors, and (c) photograph of a 100 nm device without lid.

Oldham and McGarrity [12] noted a strong dose enhancement effect with a 10 keV X-ray generator in MOS capacitors with Al metallization, we have decided to investigate in this work MOS capacitors with Aluminum metallization. We will show that dose enhancement effects can be reduced compared to [12] because the high-energy generator used in this work produces a spectra with a smaller proportion of <20 keV photons than the 10 keV generator in [12]. In addition, the use of filters makes it possible to limit the proportion of these low-energy photons even further.

In the present work, we decided to pursue the comparison between high energy X-rays and Co-60 irradiations by studying MOS capacitors. The MOS capacitor studied in this work is a very simple  $\mathrm{Si/SiO_2}$  structure where only one metallization layer is deposited on the oxide. Aluminum (Z=13) was chosen for the metallization layer to reduce dose enhancement as much as possible.

The objectives of this work are the following: 1) show that the approach used in [7] and validated on MOS and bipolar transistors (the use of a high energy X-ray generator with a lead filter) is also applicable for MOS capacitors and 2) show that for a device with a minimum of layers above the sensitive area (only one aluminum layer on the top of the oxide) an high energy X-ray irradiation with a lead filter gives the same degradation as a Co-60 irradiation.

In Section II, the experimental setup will be described. The investigated MOS capacitors and the irradiation facilities will be presented. Experimental results will be given in Sections III and IV. The effect of annealing, package lid, and bias are studied. Discussion of the obtained results and conclusion are given in Section V.

## II. DESCRIPTION OF THE EXPERIMENTAL SETUP

In this section, the investigated MOS capacitors are described and the irradiation facilities are presented.

## A. MOS Capacitors

Specific capacitors have been manufactured for this study. This allows to control the manufacturing parameters (area, oxide and metallization thicknesses, doping). These samples were fabricated at Laboratory for Analysis and Architecture of Systems (LAAS) through the RENATECH network [20] in Toulouse (France). Two different dies with two SiO<sub>2</sub> oxide

TABLE I MOS CAPACITOR PARAMETERS

Parameter	400 nm Large	400 nm Small	100 nm Large	100 nm Small
Size (mm²)	2x2	1x1	1x1	0.5x0.5
Area (mm²)	4.00	1.00	1.00	0.25
Al thickness (μm)	1.00	1.00	1.00	1.00
Ox. thickness (nm)	400.00	400.00	100.00	100.00
Ox. capacitance (pF)	345.15	86.29	345.15	86.29
SC thickness (µm)	525.00	525.00	525.00	525.00
SC capacitance (pF)	78.8	19.7	19.7	4.9

TABLE II
IRRADIATION CONDITIONS

Condition #	Source #	Filter #	Dose Rate Gy(Air)/h	length Source- target (mm)
1	Cobalt-60	None	5,28	330
2	Cobalt-60	None	0,62	920
3	Cobalt-60	None	0,15	1920
4	X-ray 320 kV 1.6 mA	2mm Al	30	400
5	X-ray 320 kV 11.4mA	2mm Al + 1mm Pb	30	400

thicknesses: 400 nm [see Fig. 1(a)] and 100 nm [see Fig. 1(b)] were manufactured on a p-type silicon substrate with a doping concentration between  $1.1 \times 10^{15}$  and  $1.6 \times 10^{15}$  at.cm<sup>-2</sup> of 525  $\mu$ m giving the Substrate Capacitance (SC). For each thickness (on each die) two capacitors of two different areas were designed. Twenty dies of each thickness are available for this study, which corresponds to 160 MOS capacitors. Each die was then mounted in a Dual InLine (DIL) package to facilitate irradiation and measurement, as shown in Fig. 1(c). On the top of the oxide, contact metallization is realized with 1  $\mu$ m aluminum layer. All the MOS capacitor parameters are given in Table I.

# B. Irradiation Facilities

All devices were irradiated with the PlatfoRm for the Study of the Effects of Ionizing Radiation on Electronics (PRESERVE) at the Institute of Electronics and Systems (IES), Montpellier, France. Two irradiation facilities are used in this work: a 60 curies Co-60 source and an 320 kV X-RAD320 X-ray generator. For dosimetry, two cross-calibrated (in Air) ionization chambers from PTW are used to measure dose rates: the TM30013 (with a 30 keV to 50 MeV energy range) connected to the Unidos E dosimeter for Co-60, and the TM7862 (with a 7.5 to 420 KeV energy range) for the X-ray. In this article, the dose has been corrected as a function of the energy spectrum of the facility and is given in Gy(SiO<sub>2</sub>) [7].

The irradiation conditions are given in Table II. Five irradiation conditions are considered: Co-60 irradiation with three different dose rates, 320 kV X-rays irradiation with Al filter, and X-rays irradiation with Al + Pb filter. The Al filter allows to attenuate low energies below 15 keV so when we perform the dose rate measurement for X-ray with the Al filter, we are not limited by the TM7862 chamber whose

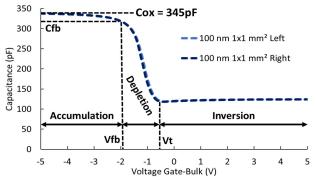


Fig. 2. Standard CV on two 100 nm MOS capacitors with an area of  $1 \times 1 \text{ mm}^2$ .

limit is 7.5 keV. In our case the Co-60 source is a panoramic irradiator in a large room, which greatly reduces secondary photon generation, so filters are use for condition 1 to 3.

It is also important to be in electronic equilibrium when testing total dose. This is difficult to achieve with commercial components due to the unknown BEOL. Our capacitors have the advantage of being metallized in Al (low Z), which reduces the effects of dose enhancement [21].

Finally, it is essential to compare the degradation of components at equivalent doses. To do this we use conversion factors from dose (air) to (SiO<sub>2</sub>). Knowing the spectrum generated, the dosimetry [Gy(Air)] and the target (in SiO<sub>2</sub>). We can calculate a SiO<sub>2</sub> dose by correlating each spectrum with the mass energy-absorption coefficient ( $\mu$ en/ $\rho$ ) obtained from NIST database, as detailed in [7]. Factors are: Co-60:1; Xray with Al filter: 2,25; Xray with Al + Pb filter: 1,15.

#### III. IRRADIATION RESULTS

In this section, the experimental data obtained on MOS capacitors submitted to Co-60 and X-Ray irradiation are given.

#### A. MOS Capacitors Characterization

Capacitance–Voltage (CV) characterizations were performed with B1500 semiconductor device parameter analyzer from Keysight. These measurements were made at a frequency of 1 MHz with 30 mV oscillations. The measurement voltage range was limited from -5 to 5 V to reduce the risk of oxide capacitor breakdown. The voltage range was applied in the direction from -5 to 5 V by step of +0.2 V each 100 ms.

It is well known that for an MOS capacitor, the capacitance changes with an applied dc voltage between the gate and bulk (Vgb). As a result, the modes of operation of the MOS capacitor change as a function of the applied voltage. In Fig. 2, a standard CV is plotted, before irradiation, for two 100 nm MOS capacitors (on the same die) with an area of  $1 \times 1 \text{ mm}^2$  (the blue and the orange dashed lines). As the voltage increases from -5 to 5 V, the MOS capacitor passes through accumulation, depletion, and inversion modes [22], [23], [24]. For a p-type MOS capacitor, the oxide capacitance (Cox) is measured in the strong accumulation region where the voltage is negative enough that the capacitance is constant and the CV curve is flat. For example, in Fig. 2, the Cox value is 345 pF which is close to our theoretical values given in Table I (345.15 pF for 100 nm and  $1 \times 1 \text{ mm}^2$ ).

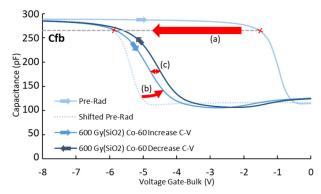


Fig. 3. Standard TID effect on CV for a MOS capacitor. 100 nm capacitor with an area of  $1 \times 1 \text{ mm}^2$  irradiated in condition 2 (Co-60) (see Table II) for a 600 Gy(SiO<sub>2</sub>) total dose.

Another important parameter is the flatband voltage  $V_{\rm fb}$ . Flatband voltage and its shift (after irradiation) are widely used to extract oxide charges. The flatband voltage can be extracted from the CV curve thanks to the capacitance method [22]: the flatband capacitance Cfb is calculated from Cox and the Debeye length, this Cfb capacitance is used to determine on the CV curve the flatband voltage as depicted in Fig. 2.

## B. Irradiation of MOS Capacitors

MOS capacitors (all oxide thickness and all area) were irradiated in the five conditions given in Table II. An example is plotted in Fig. 3. In this figure, a 100 nm capacitor with an area of  $1 \times 1 \text{ mm}^2$  is irradiated in condition 2 for a 600 Gy(SiO<sub>2</sub>) total dose. The light blue solid curve corresponds to the prerad CV and the dark blue curve corresponds to the CV after 600 Gy(SiO<sub>2</sub>). The darker blue curve is identical to the dark blue curve, but the CV measurements were performed with decreasing Vgb. A dashed blue curve repeats the prerad curve, but shifted, to highlight the change in slope.

From this Fig. 3, the three main effects of TID on the CV curve can be identified [22]. The first one corresponds to the shift of the flatband voltage (illustrated by the red arrow (1) in Fig. 3), and is due to oxide-trapped charges. The second one corresponds to a widening of the depletion region, i.e., a reduction of the slope of the CV curve (illustrated by the red arrow (2) in Fig. 3), and corresponds to interface trapped charges. The last red arrow (3) shows the mobile charges in the interfacial zone due to impurities. These three main effects will be used in the remainder of this article to characterize the degradation.

For each irradiation condition, 2 DIP packages were used: one with a 100 nm oxide thickness and a second one with a 400 nm oxide thickness. Each package contains 4 capacitors with a fixed oxide thickness (100 or 400 nm). These four capacitors are divided into pairs, two large surface area capacitors and two small surface area capacitors for each package. This gives an average of two capacitors with the same data sheet per irradiation condition. For each irradiation condition, it gives eight capacitors.

Fig. 4 details all the CVs achieved for one irradiation condition, each CV being the average of two capacitors as explained previously.

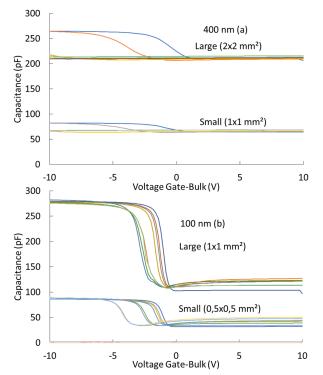


Fig. 4. Dose effect for irradiation condition 2 (Co-60) on (a) 400 nm and (b) 100 nm MOS capacitor with large and small area.

The charge trapping in the oxide is clearly visible for both oxide thicknesses. The thicker the oxide, the more flatband voltage shift. Fig. 4(a) shows that from the second measurement the flatband voltage is outside the reading range of the B1500 ( $\pm 10~\rm V$ ) for the 400 nm capacitors, whereas the 100 nm capacitors remain analysable for all the steps made. We can also see that the slopes remain mostly parallel this indicates a low presence of trapped charge at the interface. Finally, the inversion zone is not perfectly linear for some of our CVs. The frequency chosen to carry out the CVs was not high enough. This will not be a problem for the rest of the study, as no parameter is extracted from this part of the curve.

The high oxide thickness of the 400 nm capacitor makes them more sensitive to dose deposition, resulting in greater degradation for the same dose. 400 nm capacitors are not adapted to our irradiation facilities. We can work with minimum steps of 10 Gy(1 krad). Therefore, in order to ensure a more reliable analysis, we will focus on the study of 100 nm capacitors of  $1 \times 1$  and  $0.5 \times 0.5$  mm<sup>2</sup>.

For the first part of the results analysis, all the components are irradiated at room temperature, and a maximum fixed time of 40 min has been defined to characterize the components and so limit annealing. It is well known that the degradation of such components is greater when a bias is applied during irradiation. Since the degradations obtained are already significant and enable us to highlight the desired effects, we chose not to apply a bias for this part to the MOS capacitor during irradiation.

A first detailed example is given in Fig. 5, where a 100 nm MOS capacitor with an area of  $1 \times 1 \text{ mm}^2$  is irradiated in condition 2 up to 253 Gy(SiO<sub>2</sub>).

Fig. 5 shows up the fact that at room temperature and with all the pins at ground, the main phenomenon is the shifting of

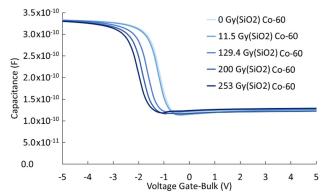


Fig. 5. Dose effect for irradiation condition 2 (Co-60) on a 100 nm MOS capacitor with an area of  $1 \times 1 \text{ mm}^2$  from 0 to 253 Gy(SiO<sub>2</sub>), unbiased.

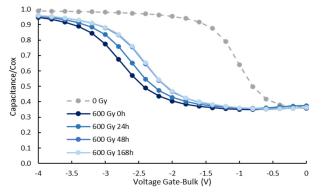


Fig. 6. Annealing effect for irradiation condition 2 (Co-60) at 590 Gy(SiO<sub>2</sub>) on a 100 nm MOS capacitor with an area of  $0.5 \times 0.5$  mm<sup>2</sup>.

the  $V_{\rm fb}$  toward the left. This parameter will be extracted for the Co-60/X-rays comparaison.

# C. Annealing

Since the X-rays irradiations are shorter than the cobalt irradiations, it is important to investigate annealing effects. Room temperature annealing have been then performed after X-rays irradiations. The obtained results are presented in Figs. 6 and 7. For each irradiation condition presented above, measurements were taken 24, 48, and 168 h after the last total dose step to study annealing at room temperatures. The devices used in Figs. 6 and 7 were irradiated at 590 Gy(SiO<sub>2</sub>) with Co-60 under condition 2. 15% annealing is observed and the majority of annealing takes place during the first 48 h. There is less than 2% variation between 48 and 168 h.

We have seen that after one week of annealing at room temperature, the annealing effect is less than 2%. These measurements were therefore repeated for each experiment and then averaged. An average annealing of around +0.3 V for flatband voltage at 168 h was measured for Co-60 (conditions 1–3) and for aluminum-filtered X-rays (condition 4). For X-rays filtered with aluminum + lead (condition 5), the average annealing at 168 h was only +0.12 V. This is explained by the total dose received (and so degradation) being 2 times lower, only 253 Gy compared with 600 Gy for conditions 2–4. We also extracted the standard deviation of the anneals to form the error bars which are stable whatever the dose deposited and conditions. These standard deviations are mainly due to the initial values of the capacitors.

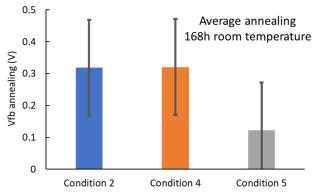


Fig. 7. Annealing effect for irradiation condition 2 (Co-60) 4 and 5 (X-rays) at 590  $Gy(SiO_2)$  for 1 and 4, and 253  $Gy(SiO_2)$  for condition 5 (Xray-Al + Pb). Error bars corresponds to three standard deviations.

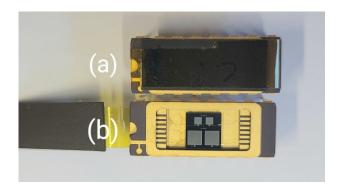


Fig. 8. Two photographs of 400 nm devices (a) with and (b) without lid.

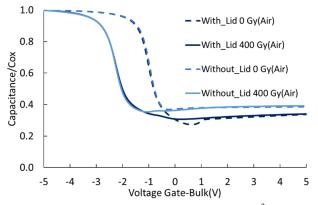


Fig. 9. Comparaison of normalized CV of 100 nm  $1\times 1$  mm<sup>2</sup> at 0 (dashed) and 400 (solid) Gy(Air) with irradiation condition 2 (Co-60) lid (dark blue) and without lid (light blue).

# D. Package Lid

Our components are delivered with a generic lid. In order to investigate the effect of such a lid, irradiations have been performed with and without lid. The case is a generic ceramic plate 1 mm thick which covers all the capacitors (see Fig. 8).

Experimental results are presented in Fig. 9 for 100 nm  $1 \times 1 \text{ mm}^2$  MOS capacitors irradiated with Co-60 (in condition 2). After irradiation, no significant difference is observed between the MOS capacitors irradiated with a lid (blue curves) and the ones irradiated without lids (oranges curves) in terms of  $V_{\rm fb}$  variation. Measurements show a small gap for the  $V_{\rm fb}$  and a major difference in the inversion zone. These deviations are mainly due to the gap between each device.

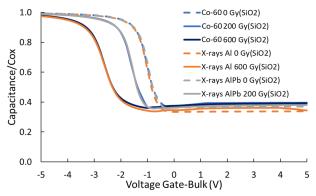


Fig. 10. Comparison of normalized CV of 100 nm MOS capacitors with an area of 1  $\times$  1 mm<sup>2</sup> irradiated in condition 1 (Co-60) at 0–200–600 Gy(SiO<sub>2</sub>), 4 at 0–600 Gy(SiO<sub>2</sub>), and 5 at 0–200 Gy(SiO<sub>2</sub>) (X-rays).

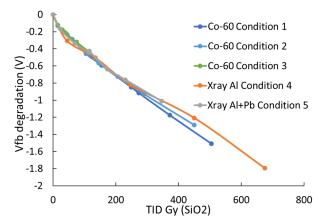


Fig. 11. Comparison of the five irradiation conditions on 100 nm MOS capacitors with an area of 1  $\times$  1 mm $^2.$ 

## E. Comparaison Between all Irradiation Conditions

It is difficult to compare the CV curves for different conditions due to the scattering of the results before irradiation. Therefore, we will use the normalized capacitance C/Cox to compare the results for different conditions.

In Fig. 10, the comparison of irradiation conditions 1 (Co-60), 4 and 5 (X-rays) is shown for a 100 nm capacitor with an area of  $1 \times 1 \text{ mm}^2$  and for a 0–200–600 Gy(SiO<sub>2</sub>) total dose. The curves obtained after irradiations are very close, which means that Co-60 irradiation, X-ray irradiation with Al filter, and X-ray irradiation with Al + Pb filter lead to the same observable degradation for high frequency CV unbiased.

In order to generalize this result, that is to say to carry out the comparison of all the irradiation conditions for several MOS capacitors which we studied, we chose to represent in Figs. 11 and 12 the shift of the flatband voltage as a function of the dose. For the following curves, the data displayed corresponds to the average of measurements taken on pairs of capacitors with identical physical parameters. In Fig. 11, the flatband shift as a function of the dose is plotted for a 100 nm MOS capacitor with an area of  $1 \times 1 \text{ mm}^2$ . It is important to note that in Fig. 11 no particular difference between the several irradiation conditions is observed. We can also note that the variation of the flatband voltage is important, which corresponds to a strong charge trapping in the oxide.

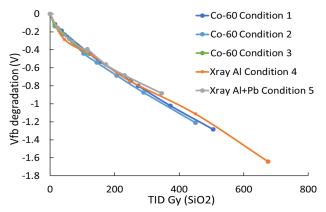


Fig. 12. Comparison of the five irradiation conditions on 100 nm MOS capacitors with an area of 0.5  $\times$  0.5  $\text{mm}^2.$ 

The same results can be observed in Fig. 12, where the flatband shift as a function of the dose is plotted for a 100 nm MOS capacitor with an area of  $0.5 \times 0.5$  mm<sup>2</sup>.

The same comparison of all the irradiation conditions has been done for the reduction of the slope of the *CV* curve. All the curves exhibit the same trend, no particular difference can be made between the several irradiation conditions and the reduction is weak, i.e., the interface trapped charge is weak.

As expected, since both the large area and the small area capacitors share the same oxide parameters, large and small capacitors show identical flatband voltage degradation. The differences in results between the  $100 \text{ nm } 1 \times 1 \text{ mm}^2$  and  $0.5 \times 0.5 \text{ mm}^2$  capacitors are completely contained within the error bars of 3 standard deviations (see Fig. 13).

The same comparison of all the irradiation conditions has been done for the reduction of the slope of the *CV* curve. All the curves exhibit the same trend, no particular difference can be made between the several irradiation conditions and the reduction is weak, i.e., the interface trapped charge is weak.

#### IV. BIASED IRRADIATION RESULTS

We are now going to study the different irradiation conditions effects while applying a voltage of 1 MV/cm on the capacitor gates. This means applying Vgb = +10 V for 100 nm and Vgb = +40 V for 400 nm. This bias should limit the differences in charge yields between the different conditions and a more rapid degradation of  $V_{\rm fb}$  is expected. This will further limit the use of 400 nm capacitors, which are already very difficult to operate without bias. Moreover, knowing that the degradation was going to be more important, the CVs were extended to  $\pm 10$  V and slowed down to allow more precision. This allowed us to obtain a standard deviation of 0.2 V for the measurements in this section.

#### A. Flatband Voltage

For each irradiation condition an additional unbiased 100 nm CMOS die was added. Results have been extracted for this unbiased component and are similar to the results in Section III. This confirms the previous results and allows an unbiased reference to be made in relation to the biased components. A curve corresponding to the trend found in Section III-E is therefore displayed in green.

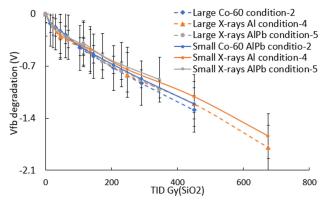


Fig. 13. Comparison of the three irradiation conditions [2(Co-60) and 4-5(X-Rays)] on 100 nm MOS capacitors with area of  $0.5 \times 0.5$  mm<sup>2</sup> (Small) and  $1 \times 1$  mm<sup>2</sup> (Large). Error bars corresponds to three standard deviations.

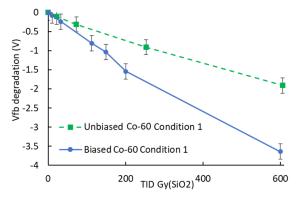


Fig. 14.  $V_{\rm fb}$  degradation versus TID Gy(SiO<sub>2</sub>) with condition 1 (Co-60) for 100 nm 1  $\times$  1 mm<sup>2</sup> MOS capacitor biased (+10 V) and unbiased. Error bars corresponds to three standard deviations.

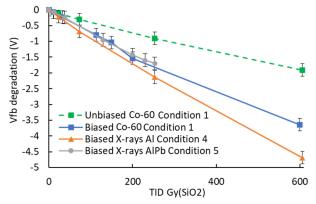


Fig. 15. Comparison for three irradiation conditions [1(Co-60)-4-5(X-Rays)] of 100 nm MOS capacitors with area of  $1 \times 1 \text{ mm}^2$  biased and unbiased. Error bars corresponds to three standard deviations.

In Fig. 14 are shown results of  $V_{\rm fb}$  drift versus TID for biased component. As expected, we end up with an increase in  $V_{\rm fb}$  shift compared to the unbiased component (green). Biasing electronic components limits initial recombination and therefore increases the number of trapped charges in the oxide during irradiation. With a bias of 1 MV/cm, the  $V_{\rm fb}$  voltage shift is multiplied by  $\sim$ 2.

The objective of the study is to investigate the differences between all the proposed irradiation conditions. Fig. 15 details the degradation of  $V_{\rm fb}$  as a function of dose for different conditions. It can be seen that the biased components were all more degraded than the unbiased results. But unlike the

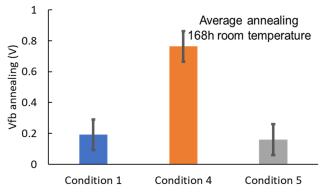


Fig. 16. Comparison of the  $V_{\rm fb}$  annealing for 168 h at room temperature for three irradiation conditions [1(Co-60)-4-5(X-Rays)] on 100 nm MOS capacitors with area of  $1 \times 1 \ {\rm mm}^2$  biased and unbiased. Error bars corresponds to three standard deviations.

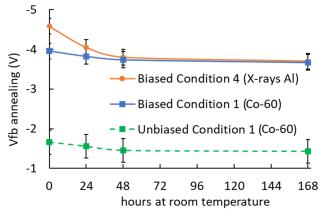


Fig. 17. Comparison of the  $V_{\rm fb}$  annealing for 0, 24, 48, and 168 h at room temperature for irradiation conditions 1 (Co-60) and 4 (X-Ray Al) after 600 Gy(SiO<sub>2</sub>) on 100 nm MOS capacitors with area of 1  $\times$  1 mm<sup>2</sup> biased and unbiased. Error bars corresponds to three standard deviations.

unbiased test, this time the results are not homogeneous. The aluminum-only X-ray generator (condition 4) does not seem to match the results for conditions 1 and 5.

The use of lead filters allows to limit the photoelectric effect by cutting the low energies photons and to get closer to Compton scattering processes as Co-60.

# B. Biased Flatband Voltage Annealing

As we noted earlier, a discrepancy appears with biased devices when irradiation conditions 4 (Al X-ray) is used. Fig. 16 shows the average annealing effect over 168 h at room temperature for the different conditions studied previously. Contrary to the results of Section III-C, a major difference appears.

For conditions 1 and 5 we find equivalent values to those found in Section III-C. Condition 5 being slightly lower due to the lower total cumulative dose (253 Gy(SiO<sub>2</sub>) in total compared with 600 Gy(SiO<sub>2</sub>) for conditions 1 and 4). Nevertheless, a large difference appears when annealing the components irradiated with condition 4: an average annealing measured almost 3 times higher (~0.3 V unbiased against ~0.8 V with bias).

Fig. 17 shows the evolution of  $V_{\rm fb}$  at room temperature from 0 to 168 h after irradiation with 600 Gy(SiO<sub>2</sub>). The biased and unbiased curves for condition 1 show an equivalent

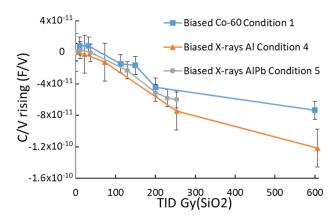


Fig. 18. Comparison of CVs hysteresis for three irradiation conditions [1(Co-60)-4-5(X-Rays)] on 100 nm MOS capacitors with area of  $0.5 \times 0.5 \text{ mm}^2$  biased. Error bars corresponds to three standard deviations.

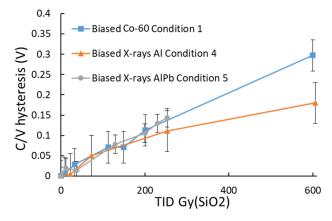


Fig. 19. Comparison of CVs hysteresis for three irradiation conditions [1(Co-60)-4-5(X-Rays)] on 100 nm MOS capacitors with area of 1  $\times$  1 mm<sup>2</sup> biased. Error bars corresponds to three standard deviations.

trend. Condition 4, which initially shows more degradation, has a much stronger annealing for the first 48 h before returning to the annealing degradation level of condition 1.

## C. Interface Charges

Applying a bias voltage of 1 MV/cm on the gate of MOS capacitor has accentuated the appearance of interface charges. The evolution of the interface charges as a function of dose for the different irradiation conditions can be seen in Fig. 18. This is similar to the trends observed in the study of generic MOS [7]. Co-60 is the least degrading on the interface charges. There is a gap between Co-60 and high-energy X-ray, but this is reduced when a lead filter is used in addition to the Al. The same trend is observed for large surface area  $(1 \times 1 \text{ mm}^2)$  and small surface area  $(0.5 \times 0.5 \text{ mm}^2)$  capacitors.

#### D. Interface charges Mobility

If we perform two CV runs, increasing then decreasing for the Vgb, we can extract a hysteresis revealing the mobility of the interface charges. Fig. 19 shows the evolution of this hysteresis as a function of the dose in  $Gy(SiO_2)$  for the following three irradiation conditions: 1 (Co-60), 4 (X-ray Al),

and 5 (X-ray Al + Pb). These results are for MOS capacitors biased at 1 MV/cm. From the point of view of mobility, the results are similar to the trend in Section IV-A. Condition 1 (Co-60) and condition 5 (X-ray AlPb) follow the same trend, whereas this time condition 4 (X-ray Al), instead of being the most degrading, turns out to be less degrading. The same trend is observed for large surface area ( $1 \times 1 \text{ mm}^2$ ) and small surface area ( $1 \times 1 \text{ mm}^2$ ) and small surface area ( $1 \times 1 \text{ mm}^2$ ) capacitors.

#### V. DISCUSSION AND CONCLUSION

In this article, a comparison between high-energy X-rays and Co-60 irradiations has been realized on MOS capacitors. *CV* characterization has been used to study the dose response of MOS capacitors.

When exposed to an ionizing dose, all the investigated devices exhibit a large shift of the flatband voltage and a weak reduction of the slope of the *CV* curve, which means that the degradation is mainly due to oxide-trapped charges than interface-trapped charges. The effects of both the annealing after irradiation and the presence of a package lid have been also investigated. It is shown that they have no significant effect on the investigated MOS capacitors.

In order to compare high-energy X-rays and Co-60 irradiations, five irradiation conditions were studied. For all the investigated devices, no particular difference between the several irradiation conditions was observed. This means that a high-energy X-ray irradiation with a lead filter leads to the same degradation as Co-60 irradiation for the investigated MOS capacitors. This result corresponds to what has been proposed in [7] with the difference that we have no gap between the degradations obtained with Co-60 and high energy X-rays with a lead filter. This lack of gap is explained by the structure of the studied components. Indeed, the MOS capacitors were manufactured with only one thin aluminum layer on the top of the oxide.

The experiments were then reproduced with bias on the gate. This highlighted the benefits of the lead filter when using a high-energy X-ray generator. The Co-60 and Al + Pb filtered X-ray results were similar, while a gap appeared in the degradation of the  $V_{\rm fb}$  with X-ray filtered only by aluminum. Finally, this also revealed the charge trapping at the interface and the charge mobility at the interface.

To take this work a step further, we'll need to run simulations with GEANT4 and irradiate a wide range of components.

## ACKNOWLEDGMENT

RADNEXT is an H2020 INFRAIA-02-2020 infrastructure project with the objective of creating a network of facilities and related irradiation methodology for responding to the emerging needs of electronics component and system irradiation; as well as combining different irradiation and simulation techniques for optimizing the radiation hardness assurance for systems, focusing on the related risk assessment.

X-ray and Co-60 tests were performed using the PRE-SERVE (Platform, which was funded by the Occitanie Region and the European Union) via European Regional Development Fund (ERDF) funds.

#### REFERENCES

- G. M. Moore and M. A. Pomper. (2015). Permanent Risk Reduction: A Roadmap for Replacing High-risk Radioactive Sources and Materials. Accessed: 2023. [Online]. Available: https://www.nonproliferation.org/wp-content/uploads/2015/07/Pomper-Moore-2015.pdf
- [2] A. Bawden. (2021). Alternatives to Radioactive Materials: A National Strategy to Support Alternative Technologies May Reduce Risks of a Dirty Bomb: Report To Congressional Committees. Accessed: 2023. [Online]. Available: https://purl.fdlp.gov/GPO/gpo171233
- [3] M. T. Itamura et al. Radiological Security Through Cesium Irradiator Replacement in the United States. Accessed: 2023. [Online]. Available: https://www.osti.gov/servlets/purl/1592558
- [4] Microcircuits, Standard MIL-STD-883, Dept. Defense, Defense Supply Center, Whitehall, OH, USA, Feb. 2017.
- [5] Total Dose Steady-State Irradiation Test Method, ESCC, ESA, ESA, Paris, France, 2007.
- [6] Standard Guide for Ionizing Radiation (Total Dose) Effects Testing of Semiconductor Devices, Standard ASTM F1892, 2018.
- [7] V. Girones et al., "The use of high-energy X-ray generators for TID testing of electronic devices," *IEEE Trans. Nucl. Sci.*, vol. 70, no. 8, pp. 1982–1989, Aug. 2023, doi: 10.1109/TNS.2023.3279626.
- [8] D. Lambert et al., "TID effects evaluation induced by photon sources in MOS devices: Impact of geometry and materials," *IEEE Trans. Nucl. Sci.*, to be published.
- [9] D. M. Fleetwood, P. S. Winokur, and J. R. Schwank, "Using laboratory X-ray and cobalt-60 irradiations to predict CMOS device response in strategic and space environments," *IEEE Trans. Nucl. Sci.*, vol. NS-35, no. 6, pp. 1497–1505, Dec. 1988.
- [10] D. M. Fleetwood, P. S. Winokur, L. C. Riewe, and R. L. Pease, "An improved standard total dose test for CMOS space electronics," *IEEE Trans. Nucl. Sci.*, vol. 36, no. 6, pp. 1963–1970, Dec. 1989, doi: 10.1109/23.45393.
- [11] D. M. Fleetwood et al., "Using a 10-keV X-ray source for hardness assurance," *IEEE Trans. Nucl. Sci.*, vol. NS-33, no. 6, pp. 1330–1336, Dec. 1986, doi: 10.1109/TNS.1986.4334601.
- [12] T. R. Oldham and J. M. McGarrity, "Comparison of 60Co response and 10 KeV X-ray response in MOS capacitors," *IEEE Trans. Nucl. Sci.*, vol. NS-30, no. 6, pp. 4377–4381, Dec. 1983, doi: 10.1109/TNS. 1983.4333141.
- [13] M. R. Shaneyfelt, D. M. Fleetwood, J. R. Schwank, and K. L. Hughes, "Charge yield for cobalt-60 and 10-keV X-ray irradiations of MOS devices," *IEEE Trans. Nucl. Sci.*, vol. 38, no. 6, pp. 1187–1194, Dec. 1991, doi: 10.1109/23.124092.
- [14] D. M. Fleetwood, P. S. Winokur, R. W. Beegle, P. V. Dressendorfer, and B. L. Draper, "Accounting for dose-enhancement effects with CMOS transistors," *IEEE Trans. Nucl. Sci.*, vol. NS-32, no. 6, pp. 4369–4375, Dec. 1985, doi: 10.1109/TNS.1985.4334126.
- [15] D. B. Brown and C. M. Dozier, "Reducing errors in dosimetry caused by low energy components of Co-60 and flash X-ray sources," *IEEE Trans. Nucl. Sci.*, vol. NS-29, no. 6, pp. 1996–1999, Dec. 1982, doi: 10.1109/TNS.1982.4336485.
- [16] T. R. Oldham, "Analysis of damage in MOS devices for several radiation environments," *IEEE Trans. Nucl. Sci.*, vol. NS-31, no. 6, pp. 1236–1241, Dec. 1984, doi: 10.1109/TNS.1984.4333489.
- [17] J. R. Schwank et al., "Correlation between co-60 and X-ray radiation-induced charge buildup in silicon-on-insulator buried oxides," *IEEE Trans. Nucl. Sci.*, vol. 47, no. 6, pp. 2175–2182, Dec. 2000, doi: 10.1109/23.903750.
- [18] P. Paillet et al., "Comparison of charge yield in MOS devices for different radiation sources," *IEEE Trans. Nucl. Sci.*, vol. 49, no. 6, pp. 2656–2661, Dec. 2002, doi: 10.1109/TNS.2002.805438.
- [19] P. Paillet et al., "Total dose hardness assurance testing using laboratory radiation sources," *IEEE Trans. Nucl. Sci.*, vol. 50, no. 6, pp. 2310–2315, Dec. 2003, doi: 10.1109/TNS.2003.821392.
- [20] RENATECH Network. Accessed: Feb. 2024. [Online]. Available: https://projets.renatech.org/
- [21] D. M. Long, D. G. Millward, R. L. Fitzwilson, and W. L. Chadsey, Handbook for Dose Enhancement Effects in Electronic Devices, document RADC-TR-83-84, Mar. 1983. Accessed: 2023. [Online]. Available: https://apps.dtic.mil/sti/pdfs/ADA128490.pdf
- [22] D. K. Schroder, Semiconductor Material and Device Characterization. New York, NY, USA: Wiley, 1998.
- [23] E. H. Nicollian and J. R. Brews, Metal Oxide Semiconductor Physics and Technology. New York, NY, USA: Wiley, 1982.
- [24] S. M. Sze and K. K. Ng, Physics of Semiconductor Devices, 3rd ed. New York, NY, USA: Wiley, 2006, p. 202, doi: 10.1002/0470068329.