

DD

## HIGH ENERGY RESOLUTION BOLOMETERS FOR NUCLEAR PHYSICS AND X-RAY SPECTROSCOPY

A.Alessandrello<sup>1</sup>, J.W.Beeman<sup>2</sup>, C.Brofferio<sup>1</sup>, O.Cremonesi<sup>1</sup>, E.Fiorini<sup>1</sup>, A.Giuliani<sup>1</sup>, E.E.  
Haller<sup>2,3</sup>, A. Monfardini<sup>1</sup>, A.Nucciotti<sup>1</sup>, M.Pavan<sup>1</sup>, G.Pessina<sup>1</sup>, E.Preitali<sup>1</sup> and L.Zanotti<sup>1</sup>

<sup>1</sup> *Dipartimento di Fisica dell'Università di Milano e Sezione di Milano dell'INFN, via  
Celoria 16, I-20133 Milan, Italy*

<sup>2</sup> *Materials Science Division, Lawrence Berkeley National Laboratory, Berkeley CA  
94720, USA*

<sup>3</sup> *Department of Materials Science and Mineral Engineering, University of California,  
Berkeley CA 94720, USA*

### ABSTRACT

Two bolometers composed of tin absorbers and NTD Ge thermistors have been fabricated in preparation for experiments in nuclear and subnuclear physics. Both detectors fully resolve the two  $K_{\alpha 1}$  and  $K_{\alpha 2}$  lines of  $^{55}\text{Mn}$ . The deconvolved FWHM resolution in this energy region ranges from 4.5 to 5.7 eV, for different published values of intrinsic widths and asymmetries of these lines, the best ever obtained at this energy with any energy dispersive detector. The  $K_{\beta'}$  satellite peak is analyzed for the first time in a measurement with an energy dispersive spectrometer.

PACS codes: 29.40.Vj, 29.30.Kv, 07.85.Nc, 07.20Mc

To be published in Physical Review Letters



Measurements of low energy events (a few keV) in nuclear and subnuclear physics are attracting great interest. Typical examples are the studies of low energy beta decays in view of the determination of the electron antineutrino mass [1,2]. In astrophysics high resolution X-ray spectroscopy in the region between 0.1 and 10 keV [3] is of considerable interest, for instance, in astronomical observations of X-rays emitted thermally by interstellar or intergalactic gas. From a more general point of view high resolution X-ray spectroscopy has numerous applications in atomic physics and material science [4].

Low energy X-ray spectroscopy is mainly performed with wavelength dispersive spectrometers (WDS) instrumented with Bragg crystals. This method yields an excellent energy resolution, but poor efficiency since only a narrow band of energy can be analyzed at a time. The complementary energy dispersive spectroscopy is mainly performed with Si (Li) semiconductor detectors, whose best resolution in the energy region of a few keV is of  $\sim 120$  eV FWHM [5]. Thermal detectors operated at low temperature can obtain resolutions better by at least an order of magnitude. This technique has been suggested in 1984 [6,7] and is now widely applied [8-10]. At low temperatures the heat capacity of a diamagnetic and dielectric crystal or of a superconductor well below the transition temperature is expected to be proportional to the cube of the ratio between the operating and the Debye temperature. As a consequence even the tiny energy delivered by a single particle can be measured from the resulting temperature increase by a suitable thermal sensor. The best resolution obtained so far with this type of energy dispersive spectrometers in the typical regions of  $K_{\alpha}$  and  $K_{\beta}$  lines of  $^{55}\text{Mn}$  (5.9 and 6.5 keV, respectively) ranges from 7 to 8 eV FWHM [3,11,12].

The two microbolometers described here offer a considerably improved resolution and represent the most resolving detectors constructed so far for this energy region.

A series of measurements [13] has been performed in a dilution refrigerator to optimize the performance of microcalorimeters made by thin tin absorber and Si:P and Neutron Transmutation Doped (NTD) Ge thermistors [14]. In order to be able to operate at the same time several bolometers we have implemented a multiple pre-amplifying system. It consists of ten silicon J-FET's operating at a temperature of  $\sim 120$  K near the detector in order to reduce parasitic capacitances. The required high temperature for FET operation is achieved by means of a proper thermal decoupling between the FET supporting structure and the cold point. The heat dissipated to reach the desired FET temperature, of the order of a few mW, flows to the 1.2 K stage of the dilution refrigerator.

The resolution obtained with the Si:P thermistors on the  $^{55}\text{Mn}$  lines is reasonable (13.5 eV FWHM), but the implantation-compensation procedure is not yet optimized.

Better results have been achieved with two microbolometers made by NTD Ge thermistors of  $300 \times 100 \times 20 \mu\text{m}^3$  glued to tin absorbers of  $\sim 250 \times 250 \mu\text{m}^2$  surface and 25  $\mu\text{m}$  thickness. Two 17  $\mu\text{m}$  diameter, 2 mm long aluminum wires are ultrasonically bonded to two gold pads on the NTD Ge thermistors. The pads are placed on the same  $300 \times 100 \mu\text{m}^2$  side of the thermistor and are separated by 200  $\mu\text{m}$ . The wires provide both the electrical contact and the mechanical suspension of the devices.

The two detectors are operated at about 70 mK. At this temperature the thermistor resistance was 60 M $\Omega$  and its sensitivity of about 4 M $\Omega$  /mK. The bias current was 70

pA. They were exposed to weak sources obtained by drying a 0.1 molar water solution of  $\text{NO}_3\text{H}$  with  $^{55}\text{FeCl}$  dissolved in it. The detectors give pulses with amplitude of about 200  $\mu\text{V}/\text{keV}$  and rise and decay times of  $\sim 0.5$  and  $\sim 2$  ms, respectively.

The spectra in the  $K_\alpha$  region obtained with the two microbolometers are presented in Fig. 1. The corresponding effective running times are of 26 and 71 hours, respectively. In both spectra the  $K_{\alpha 1}$  and  $K_{\alpha 2}$  lines are fully resolved for the first time with an energy dispersive spectrometer. The baseline widths of the two detectors are the same: about 3.4 eV.

The instrumental resolution of our microbolometers can be obtained by deconvolving the peaks with the Lorentzians corresponding to the intrinsic widths of the  $^{55}\text{Mn}$   $K_{\alpha 1}$  and  $K_{\alpha 2}$  lines determined in WDS measurements. In the pioneering work by the NASA-Wisconsin collaboration [3] and in the more recent experiment by E. Silver et al. [11] the Lorentzians determined by H.W. Schnopper [15] were adopted. This procedure yields intrinsic resolutions around 7.5 eV in both experiments. More precise WDS measurements of the  $K_\alpha$  doublet are, however, available and yield smaller natural widths [16-20]. A. Wollmann et al. have performed a more detailed analysis on their  $K_\alpha$  spectra obtained with a bolometer made by an Ag absorber and a transition edge strip as thermal sensor [12]. By deconvolving their  $K_\alpha$  peaks with the natural widths determined by Schnopper they obtain an instrumental gaussian resolution of  $6.4 \pm .4$  eV. This is better than the heat-pulse energy resolution itself. When using however the natural width from the WDS experiment by P.L. Lee and S.I. Salem [16] their instrumental resolution becomes  $7.2 \pm .4$  eV. In Table I we report the results of our measurements and compare them with those obtained by the most resolving energy dispersive detectors. In addition to

the deconvolution according to Shnopper we consider for our experiment the results of Lee and Salem, and the more recent ones of G. Holzer et al [20]. The instrumental resolution of our two bolometers is the same, thus indicating the reproducibility of our technique, while the long running times shows the stability of their gain.

Two peaks appear in the  $K_{\beta}$  region of  $^{55}\text{Mn}$ , as shown by Fig.2 where only the spectrum of the bolometer with a longer running time is reported. The upper one lies at 6.490 keV in agreement with the average value for the  $K_{\beta_{1,3}}$  doublet [20-21] whose separation is about 3 eV [17,20,22,23]. We are obviously unable to resolve this doublet. The presence of the satellite  $K_{\beta}'$  peak at lower energy has been already reported in WDS [15,17,22,23], but never in EDS measurements. Fitting the doublet and the satellite peak we obtain a  $K_{\beta_{1,3}}-K_{\beta}'$  energy shift of  $16 \pm 1$  eV in reasonable agreement with the above-mentioned WDS experiments.

We would like to stress that, even if the resolutions of our detectors are the best so far obtained in energy dispersive X-ray spectrometry, there is still some space for further improvements. This could be achieved for instance by a reduction of the electronic noise, by optimization of thermistor sensitivity and geometry and by a better choice of the absorber itself and/or a reduction of its thickness. It seems therefore not impossible to reach resolutions comparable to those of wavelength dispersive spectrometers with obvious advantages offered by high efficiency single quantum detectors.

The results of the measurements reported here show that energy dispersive bolometric detectors can perform X-ray spectroscopy with a resolution approaching that of Bragg crystals. This may lead to a broad range of applications in X-ray astronomy, in

fluorescence analysis of materials and even in a totally different subject like biomolecule spectroscopy [24-26]. In nuclear and subnuclear physics these microbolometers provide a powerful tool for the search for a non-zero neutrino and antineutrino mass or to detect solar neutrinos. Experiments on low energy e-captures like those of  $^7\text{Be}$ ,  $^{163}\text{Ho}$  [27], and  $^{76}\text{Ge}$  and  $^{37}\text{Ar}$  [28] or on  $\beta$  decays like that of  $^{187}\text{Re}$  [13,27] are typical examples.

We would like to express our gratitude to R. Cavallini, S. Parmeggiano M. Perego and to our student D. Losi for assistance and suggestions in the course of these measurements. Thanks are also due to G. Benedek for interesting discussions on X-ray spectroscopy, to many members of the European Network on Cryogenic Detectors and to D. McCammon for many useful suggestions. We are deeply indebted to G. Roubaud who provided us excellent sources of  $^{55}\text{Fe}$ .

This experiment has been supported in part by the Commission of European Communities under contract FRMX-CT98-0167.

## REFERENCES

- [1] Review of Particle Physics, The Europ. Phys. Journ. C 3 (1998) 1
- [2] See for instance L. Oberauer, Nucl.Phys.B (Proc. Suppl.) 70 (1998) 155
- [3] D.McCammon et al., Nucl. Instrum. and Meth. A326 (1993) 157 and references therein
- [4] M. Frank, Proc. of the VII Int. Workshop on Low Temperature Detectors, Munich 27 July-2 - Aug. 1997, ed.by S. Cooper, p.82
- [5] See for instance E. Pinotti et al., Nucl.Instrum.and Meth. A326 (1993) 85
- [6] E.Fiorini and T.O.Niinikoski: Nuclear Instrum. and Methods 224 (1984) 83
- [7] S.H.Moseley, J.C.Mather, and D.McCammon, J.Appl.Phys. 56 (1984) 1257
- [8] D. Twerenbold. Rep. Prog.Phys. 59 (1996) 349
- [9] N.Booth, B. Cabrera and E. Fiorini, Ann.Rev.Nucl.Part.Sci. 46 (1996) 471
- [10] For recent developments of cryogenic detectors see Proc. of the VII Int. Workshop on Low Temperature Detectors, Munich 27 July-2 Aug. 1997, ed.by S. Cooper
- [11] E. Silver et al., X-ray Spectrometry 25 (1996) 115
- [12] D.A. Wollmann et al., Journ.of Microscopy, 188 (1997) 196
- [13] A. Alessandrello et al., Proc. of the VII Int. Workshop on Low Temperature Detectors, Munich 27 July-2 Aug. 1997, ed.by S. Cooper, p. 138
- [14] E.E. Haller et al.: "NTD Germanium: A novel material for low temperature bolometers", Proc.Fourth.Intl.Conf.on Neutron Transmutation Doping of

Semiconductor Materials. Nat. Bureau of Standards, June 1-2, 1982. Gaithersburg, MD. R.D. Larrabee, ed., (Plenum Press 1984), p.21

- [15] H. W. Schnopper, Phys. Rev. 154 (1967) 118
- [16] P.L. Lee and S.I. Salem, Phys.Rev, A 10 (1974) 2027
- [17] S.P. Kovalczyk et al., Phys.Rev. B 11 (1975) 1721
- [18] K.S. Srivastava et al., Phys. Rev. A 25 (1982) 2838
- [19] D. Kuchler, U. Lehnert and G. Zschornack, X-ray Spectrometry 27 (1998) 177, and references therein
- [20] G. Holzer et al, Phys.Rev. 56 (1997) 4554
- [21] R.B.Firestone: Tables of Isotopes (eighth edition), Ed. by V.S. Shirley, John Wiley and Sons, INC.1996
- [22] S.I. Salem and G.M. Hockney, Phys.Rev. A 13 (1976) 330.
- [23] For a similar detailed WDS study on copper see M. Deutsch et al., Phys.Rev. A51 (1995) 283
- [24] D. Twerenbold, Nucl. Instrum. And Meth, A 370 (1996) 253
- [25] D. Gerber et al., Proc. of the VII Int. Workshop on Low Temperature Detectors, Munich 27 July-2 Aug. 1997, ed.by S. Cooper, p.73
- [26] S.E. Labov et al., Proc. of the VII Int. Workshop on Low Temperature Detectors, Munich 27 July-2 - Aug. 1997, ed.by S. Cooper, p.82
- [27] F. Gatti et al., Proc. of the VII Int. Workshop on Low Temperature Detectors, Munich 27 July-2 Aug. 1997, ed.by S. Cooper, p. 167



- [28] J. Hoehne et al., Proc. of the VII Int. Workshop on Low Temperature Detectors,  
Munich 27 July-2 Aug. 1997, ed.by S. Cooper, p. 184

TABLE I: Instrumental resolution (FWHM) of the most resolving energy dispersive spectrometers on the  $K_{\alpha}$  lines of  $^{55}\text{Mn}$  (eV)

Experiment	Deconvolution with WDS data of ref. [14]	Deconvolution with WDS data of ref. [15]	Deconvolution with WDS data of ref. [20]
McCammon et al. [3]	$7.3 \pm .4$		
Silver et al. [11]	$7.1 \pm .7$		
Wollmann et al. [12]	$6.4 \pm .4$	$7.2 \pm .4$	
This exp. (Bolometer 1)	$4.5 \pm .2$	$5.5 \pm .2$	$5.2 \pm .2$
This exp. (Bolometer 2)	$4.9 \pm .1$	$5.7 \pm .1$	$5.4 \pm .1$

## FIGURE CAPTIONS

Fig.1: Spectrum obtained with the two bolometers in the  $K_{\alpha}$  region. Bolometer 1 and 2 have been operated for 26 and 71 hours of effective running times, respectively

Fig.2: Spectrum obtained with the second bolometer in the  $K_{\beta}$  region

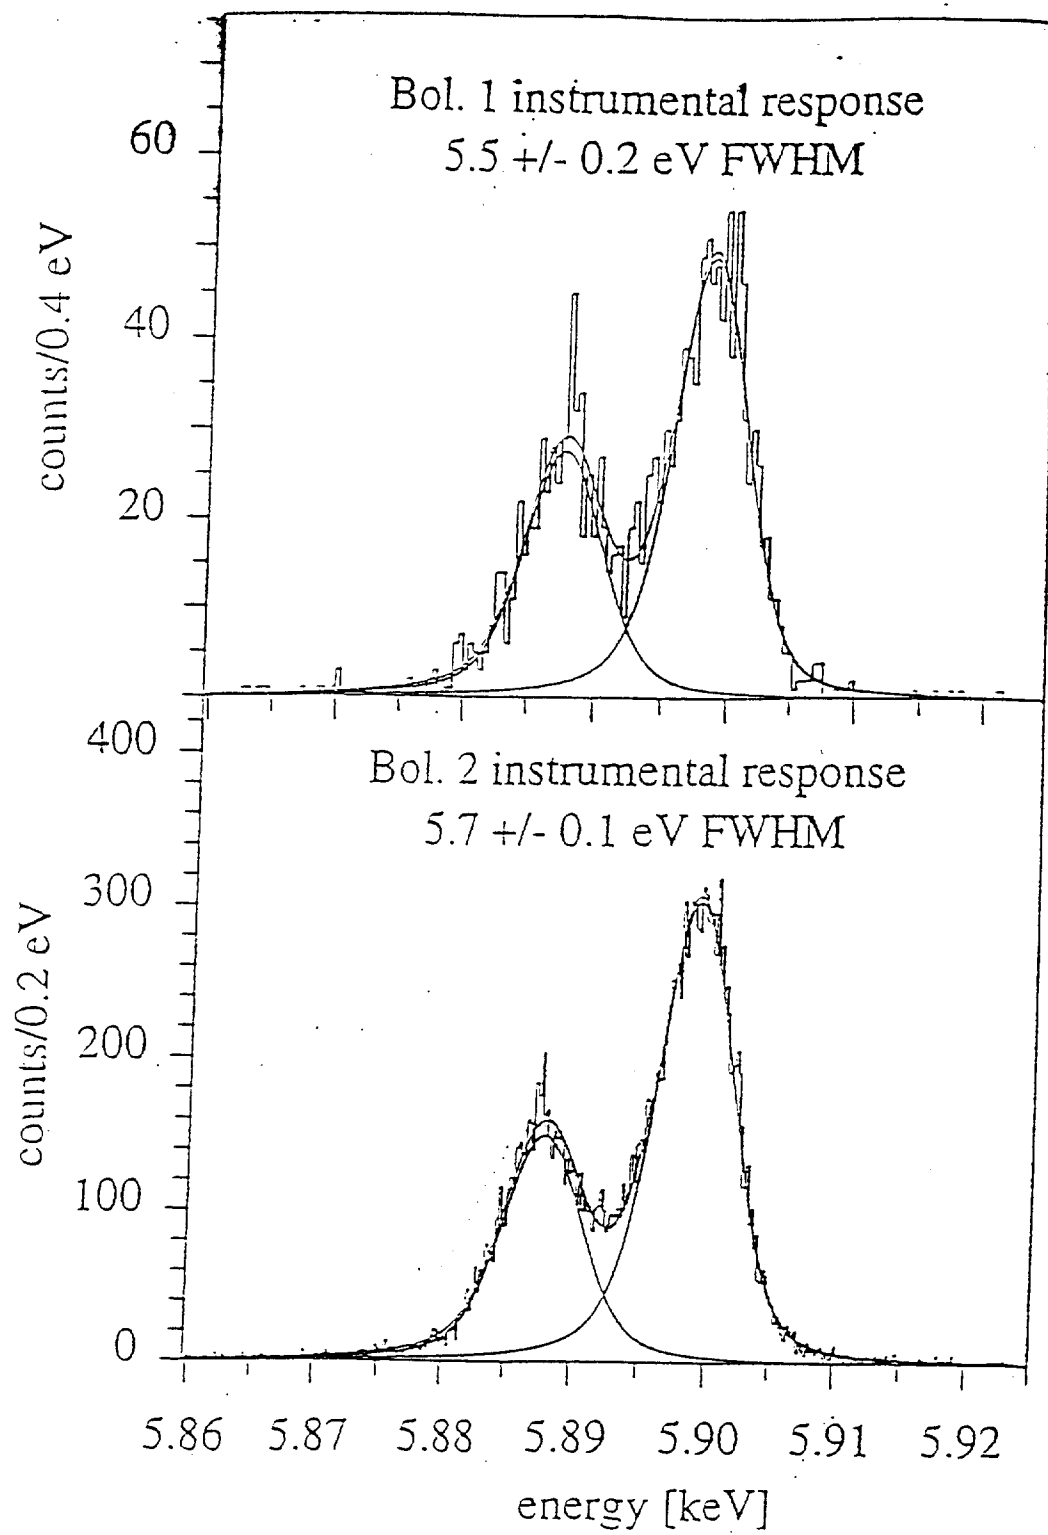


Fig. 1

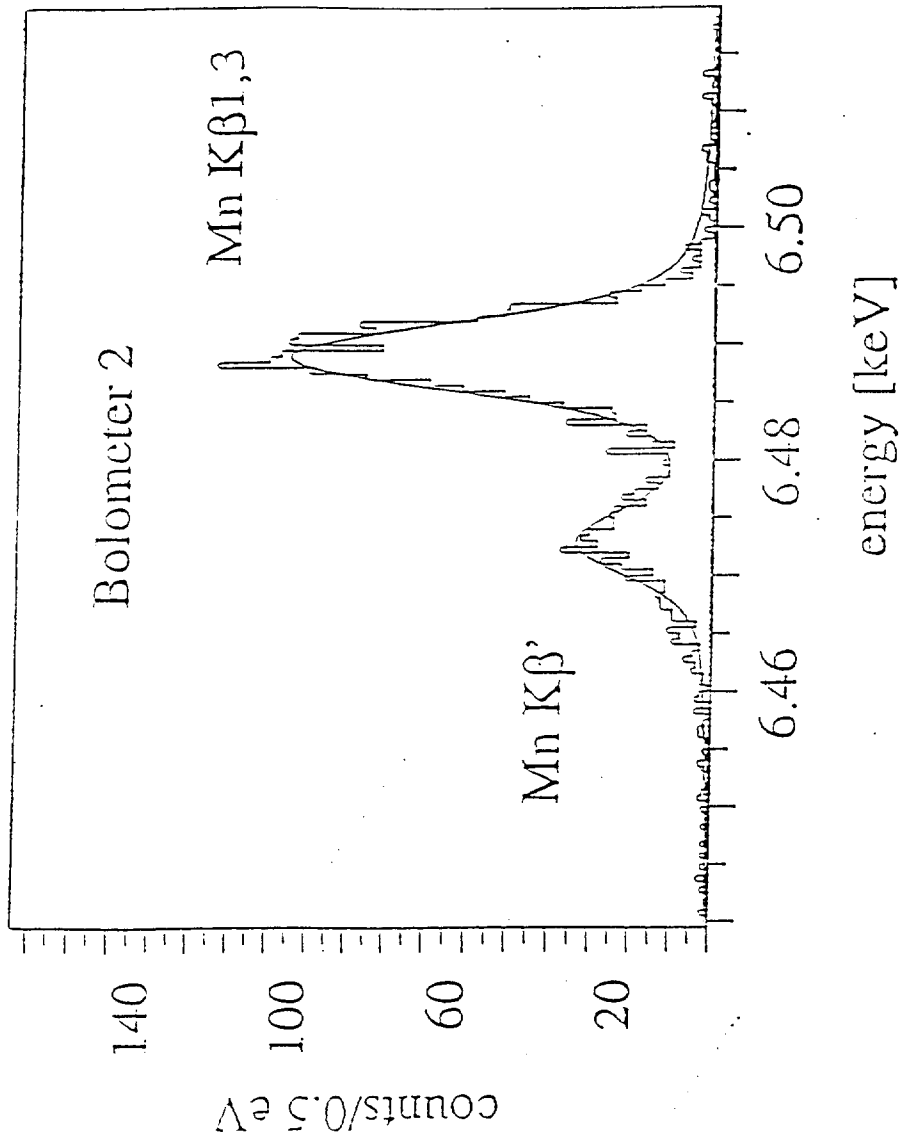


Fig. 2

