

RESEARCH

Performance assessment of the 2γ positronium imaging with the total-body PET scanners

P. Moskal¹, D. Kisiełewska^{1*}, Z. Bura¹, C. Chhokar¹, C. Curceanu², E. Czerwiński¹, M. Dadgar¹, K. Dulski¹, J. Gajewski³, A. Gajos¹, M. Gorgol⁴, R. Del Grande², B. C. Hiesmayr⁵, B. Jasińska⁴, K. Kacprzak¹, A. Kamińska¹, Ł. Kapłon¹, H. Karimi¹, G. Korcyl¹, P. Kowalski⁶, N. Krawczyk¹, W. Krzemień⁷, T. Kozik¹, E. Kubicz¹, P. Małczak⁸, M. Mohammed^{1,9}, Sz. Niedźwiecki¹, M. Pałka¹, M. Pawlik-Niedźwiecka¹, M. Pędziwiatr⁸, L. Raczyński⁶, J. Raj¹, A. Ruciński³, S. Sharma¹, Shivani¹, R. Y. Shopa⁶, M. Silarski¹, M. Skurzok^{1,2}, E. Ł. Stępień¹, S. Vandenberghe¹⁰, W. Wiślicki⁷ and B. Zgardzińska⁴

*Correspondence:

dk.dariakisiełewska@gmail.com

¹Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, prof. Stanisława Łojasiewicza 11, 30-348 Cracow, Poland

Full list of author information is available at the end of the article

Abstract

Purpose: In living organisms the positron-electron annihilation (occurring during the PET imaging) proceeds in about 30% via creation of a metastable ortho-positronium atom. In the tissue, due to the pick-off and conversion processes, over 98% of ortho-positronia annihilate into two 511 keV photons. In this article we assess the feasibility for reconstruction of the mean ortho-positronium lifetime image based on annihilations into two photons. The main objectives of this work include: (i) estimation of the sensitivity of the total-body PET scanners for the ortho-positronium mean lifetime imaging using 2γ annihilations, and (ii) estimation of the spatial and time resolution of the ortho-positronium image as a function of the coincidence resolving time (CRT) of the scanner.

Methods: Simulations are conducted assuming that radiopharmaceutical is labelled with ^{44}Sc isotope emitting one positron and one prompt gamma. The image is reconstructed on the basis of triple coincidence events. The ortho-positronium lifetime spectrum is determined for each voxel of the image. Calculations were performed for cases of total-body detectors build of (i) LYSO scintillators as used in the EXPLORER PET, and (ii) plastic scintillators as anticipated for the cost-effective total-body J-PET scanner. To assess the spatial and time resolution the three cases were considered assuming that CRT is equal to 140 ps, 50 ps and 10 ps.

Results: The estimated total-body PET sensitivity for the registration and selection of image forming triple coincidences ($2\gamma + \gamma_{\text{prompt}}$) is larger by a factor of 12.2 (for LYSO PET) and by factor of 4.7 (for plastic PET) with respect to the sensitivity for the standard 2γ imaging by LYSO PET scanners with AFOV = 20 cm. The spatial resolution of the ortho-positronium image is comparable with the resolution achievable when using TOF-FBP algorithms already for CRT = 50 ps. For the 20 min scan the resolution better than 20 ps is expected for the mean ortho-positronium lifetime image determination.


Conclusions: Ortho-positronium mean lifetime imaging based on the annihilations into two photons and prompt gamma is shown to be feasible with the advent of the high sensitivity total-body PET systems and time resolution of the order of tens of picoseconds.

Keywords: PET; positronium imaging; total-body PET; medical imaging

1 Background

In the state-of-the-art positron emission tomography (PET) the density distribution of points of positron-electron annihilations is used for the determination of the image of standardised uptake value (SUV) of the radiopharmaceutical administered to the patient. The current PET diagnostics does not take advantage of the fact that positron and electron may form a positronium atom. Yet, in up to about 40% cases^{1,2}, positron-electron annihilations inside the human body proceeds via the creation of the metastable positronium atom which in turn in quarter of cases appears as para-positronium (pPs) decaying to two photons and in three quarter of cases as ortho-positronium (oPs) decaying in vacuum into three photons. When trapped in the body, the ortho-positronium creation probability and mean lifetime strongly depend on the tissue's nanostructure and the concentration of bio-active molecules (e.g. free radicals, reactive oxygen species, and antioxidants) which can interact with the emitted positrons as well as with the formed positronium¹. In particular ortho-positronium lifetime depends significantly on the size of free volume between atoms whereas its formation probability depends on their concentration. While both lifetime and formation probability depend on the concentration and type of biofluids and bio-active molecules³. Therefore, these ortho-positronium properties may be considered as diagnostic indicators complementary to the presently available SUV index^{1,4}. Recently the in-vitro studies indicated that indeed positronium mean lifetime and its production probability as well as the average time of direct annihilation differ for healthy and cancerous uterine tissues operated from the patients^{5,6}. Another in-vitro measurements, performed with blood taken from patients before and after the chemotherapy or radiotherapy, demonstrated dependence of positronium properties in blood on the time after anti-neoplastic therapy⁷. In Figure 1, an example of the hemoglobin molecule and the main mechanisms for the positronium annihilations inside the cells is presented. The positron annihilation lifetime spectroscopy (PALS) is a well established method in the material science⁸⁻¹⁰. However, in order to make use of the positronium properties in the in-vivo medical diagnostics development of the system combining PET and PALS is required^{1,3}.

Recently, a method of positronium mean lifetime imaging, in which the lifetime, production probability and position of positronium is determined on an event-by-event basis using $oPs \rightarrow 3\gamma$ decay was described^{1,4}. The place and time of ortho-positronium decay is reconstructed by application of the trilateration technique^{11,12} which uses times and positions of registrations of three photons from $oPs \rightarrow 3\gamma$ decay. The method is applicable for radiopharmaceuticals labeled with β^+ decaying isotope emitting prompt gamma (e.g. ^{44}Sc)^{13,14}, where prompt gamma is used to determine the time of the ortho-positronium formation. The 3γ events were chosen because in case of the registration of the 3γ in principle one can reconstruct the annihilation point with better spatial precision with respect to the case when only two photons are available. It was shown¹ that for the total-body J-PET scanner, when administering to the patient a typical activity of 370 MBq, one can expect about 700 registered events per cubic centimeter of the examined patient after 20 minutes of data collection. This is a promising result however the expected statistics is rather low. Low rate of $oPs \rightarrow 3\gamma$ decays inside the tissue is due to the interaction of positronium with electrons from the surrounding atoms (pick-off process¹⁵) and due to the conversion¹⁶⁻¹⁸ of ortho-positronium into para-positronium

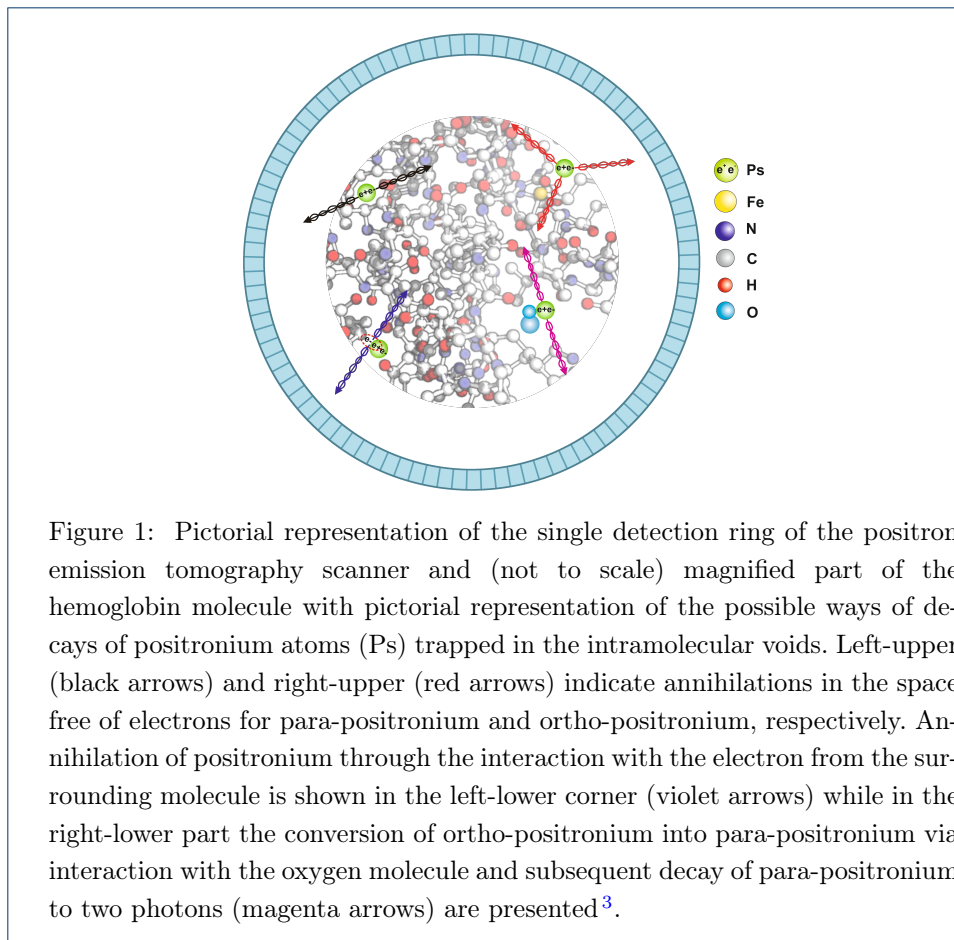

via interactions with the bio-active molecules (Fig. 1). Because of these processes the ortho-positronium lifetime decreases in the tissue to the range of few nanoseconds^{5,6} and the fraction of its decay rate into three photons $f_{oPs \rightarrow 3\gamma}$ decreases from $f_{oPs \rightarrow 3\gamma} = 1$ in vacuum to $f_{oPs \rightarrow 3\gamma} = \tau_{tissue} / \tau_{vacuum}$ in the tissue¹⁹, where τ_{tissue} and $\tau_{vacuum} = 142$ ns denote the ortho-positronium mean lifetime in the tissue and in vacuum, respectively. E.g. for $\tau_{tissue} = 2$ ns, the ortho-positronium decays 70 times more frequent to 2γ than to 3γ .

Lifetime of the decaying object may be determined by the measurement of any of its decay channels and hence the ortho-positronium mean lifetime imaging can be performed based on the $oPs \rightarrow 3\gamma$ decay¹, as well as based on the pick-off and conversion processes leading to the two back-to-back photons. In this article, we assess the feasibility of the 2γ ortho-positronium lifetime imaging for the total-body PET scanners assuming that the radiopharmaceutical is labeled with ^{44}Sc isotope emitting positrons and prompt photon with energy of 1160 keV and using two back-to-back photons for the reconstruction of the ortho-positronium decay time and decay position. The prompt photon is used to determine the time of the creation of positronium. Reconstruction of the time difference between annihilation and emission of the positron enables to disentangle between processes when para-positronium decays to two photons (black arrows in Fig. 1) and ortho-positronium converts to two photons (magenta and violet arrows in Fig. 1). The lifetime of


para-positronium (equal to 125 ps in vacuum) does not alter much as a function of properties of the tissues nanostructure (reaches about 230 ps) whereas the lifetime of ortho-positronium varies in the tissue in the range of few nanoseconds⁵ and may occur to be useful as a diagnostic indicator^{1,3}.

A statistical method of lifetime image reconstruction are yet to be conceived. Therefore, at present, in the event-by-event technique of ortho-positronium mean lifetime imaging the spatial precision of a single annihilation event reconstruction is equivalent to the spatial precision of the image. Hence, the resolution of the ortho-positronium mean lifetime image will directly depend on the time resolution of the PET detector. At present the newest TOF-PET scanners are characterized by the TOF resolution of about 210 ps²⁰ corresponding to the spatial resolution along the line of response (LOR) of about 3.8 cm. Recently a detector design with SiPM has been reported, with CRT = 85 ps for $2 \times 2 \times 3$ mm³ LSO:Ce doped with 0.4%Ca crystals and CRT of 140 ps for $2 \times 2 \times 20$ mm³ crystals with the length as used in the current PET devices²¹. Thus the TOF resolution, and consequently spatial resolution for a single event, is gradually improving by development of new crystals, SiPMs²², fast high frequency electronics²³, signals filtering²⁴ applications of the time ordered statistics^{25,26}, signal waveform sampling^{27,28} including fast and cost-effective sampling in voltage domain²⁹, and advent of machine learning techniques³⁰.

Most recently, for the single detectors 30 ps resolution was achieved which is equivalent to position resolution of 4.5 mm along the line of response³¹, and there is a continuous effort to improve it further even down to 10 ps^{23,32} which would enable to reconstruct the 2γ annihilation point with precision of 1.5 mm, where the position and time information will be directly available for each decay event. In this context it is worth mentioning that recently a new quenching circuit (QC) and single photon avalanche diode (SPAD) technology was introduced with 7.8 ps resolution³³ resulting in the resolution of 17.5 ps for the full chain of SiPM with QC and TDC³⁴.

In this article, based on the Monte-Carlo simulations, we argue that with the time resolution in the order of tens of picoseconds and the advent of the high sensitivity total-body PET systems^{35,36} the $2\gamma + \gamma_{prompt}$ mean lifetime positronium imaging based on time measurements is becoming realistic in the nearest future.

In the next section the main assumptions applied in the simulations are presented. Further on, the sensitivity for the simultaneous registration of the back-to-back photons from positronium decay and prompt photon including selection of the image forming events is estimated for the total-body PET scanners built from LYSO crystal as well as for the cost effective version of the total-body PET built from plastic scintillators. Next, results of detailed Monte-Carlo simulations of the response of the J-PET total body scanner to the point like sources arranged in the configuration as described in the NEMA norm are performed and the regular PET 2γ annihilation images as well as ortho-positronium mean lifetime images are reconstructed and compared for the three cases of assumed coincidence resolving time (CRT) of 140 ps, 50 ps and 10 ps. Finally it is shown that, owing to the large axial field-of-view of the total body scanners, the sensitivity for the positronium lifetime imaging is even larger than the present sensitivity for the 2γ metabolic imaging with

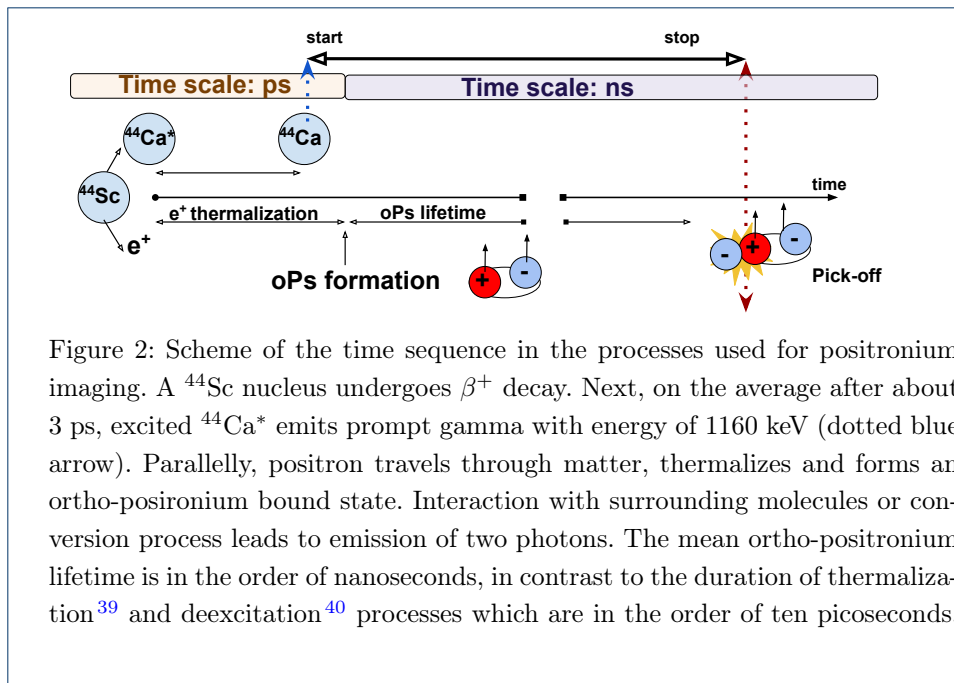

the PET scanners having 20 cm axial length, even though the discussed positronium lifetime imaging requires registration of triple coincidence events including the prompt gamma and the two back-to-back photons.

2 Materials and Methods

Positronium mean lifetime imaging may be defined as spatially resolved determination of the ortho-positronium lifetime inside the patient's body. For this purpose it is required to determine the lifetime and position of ortho-positronium on the event-by-event basis thus enabling calculation of the mean lifetime of ortho-positronium for each voxel of the image. The simulations presented in this article are conducted assuming that radiopharmaceutical is labeled with ^{44}Sc isotope which emits positron and a remaining excited daughter nucleus $^{44}\text{Ca}^*$ emits prompt gamma with energy of 1160 keV via reaction chain: $^{44}\text{Sc} \rightarrow ^{44}\text{Ca}^* e^+ \nu \rightarrow ^{44}\text{Ca} \gamma e^+ \nu$ (see Fig. 2). The single (triple coincident) event used for imaging contains three signals that carry information about the position and time of the photons' interaction in the detector: with one signal corresponding to prompt gamma and two signals corresponding to 511 keV photons originating from the annihilation of ortho-positronium while interacting with the molecular environment. The times and positions of interactions of 511 keV photons are used to determine the time and position of the annihilation point, whereas the time and position of the prompt gamma enable to determine the moment of the deexcitation of the $^{44}\text{Ca}^*$ nucleus which with the precision of tens of picoseconds³⁷ can be associated with the moment of the creation of positronium. The lifetime spectrum determined for each voxel of the patient enables to extract information about the mean ortho-positronium lifetime and its production probability^{4,38}.

2.1 Analytic estimation of sensitivity

First we performed simplified simulations in order to estimate a sensitivity for the registration and selection of triple coincidences useful for the positronium image reconstruction. In the simulation it was assumed that the PET scanner is built from the cylindrical layer of scintillator detectors. Calculations were performed for the case of the LYSO scintillators with thickness of $d = 1.81$ cm as used in the EXPLORER⁴¹ and plastic scintillators with thickness of $d = 6$ cm (two 3 cm thick layers) as optimized for the J-PET total-body prototype⁴². The two back-to-back 511 keV annihilation photons and the 1160 keV prompt photon were emitted assuming that the activity is uniform along the 200 cm long line source positioned in the central axis of the cylinder. For a single event both annihilation photons and prompt gamma were emitted from the same point. The direction of back-to-back photons and the direction of the prompt gamma were generated independently, and in both cases the isotropic distribution was assumed. The diameter of the cylinder was fixed to 80 cm whereas the length of the scanner was varied between 10 cm and 200 cm.

For a given axial field of view of the scanner the sensitivity S was calculated as a function of the AFOV using a following formula:

$$\int_{z=0}^{z=AFOV/2} dz \left[\int_{\theta_{min}(z)}^{\theta_{max}(z)} (\epsilon_{det-a}(\theta) \cdot Att_a(\theta))^2 \cdot \sin \theta d\theta \right] \left[\int_{\theta_{min}(z)}^{\theta_{max}(z)} \epsilon_{det-p}(\theta) \cdot Att_p(\theta) \cdot \sin \theta d\theta \right] \cdot \epsilon_{sel-a}^2 \cdot \epsilon_{sel-p} / L_{source}, \quad (1)$$

where θ denotes the polar angle between the photon's direction of flight and the main axis of the tomograph. $L_{source} = 200$ cm denotes the length of the annihilation line source. The detection efficiency for annihilation photons ϵ_{det-a} and prompt gamma ϵ_{det-p} were calculated as $(1 - e^{-\mu \cdot d / \sin \theta})$, where μ denotes the attenuation coefficient which for 511 keV (1160 keV) photons was assumed to be $\mu = 0.833$ cm⁻¹ (0.413 cm⁻¹) and $\mu = 0.098$ cm⁻¹ (0.068 cm⁻¹) for LYSO and plastic scintillators, respectively. $Att_a(\theta)$ and $Att_p(\theta)$ indicate attenuation in the body of annihilation photons and prompt gamma, respectively. The influence of attenuation was estimated as $e^{-\mu_{water} \cdot R_{phantom} / \sin(\theta)}$ approximating the body as a cylindrical phantom with radius of $R_{phantom} = 10$ cm filled with water with μ_{water} equal to 0.096 cm⁻¹ and 0.066 cm⁻¹ for 511 keV and 1160 keV photons, respectively. In the case of the LYSO scintillators, the selection efficiency ϵ_{sel-a} of image forming signals for 511 keV photons was estimated as a fraction of the photoelectric effect which is equal to 0.34, whereas for the plastic scintillators where 511 keV photons interact in practice only via Compton effect ϵ_{sel-a} was set to 0.44⁴³ which results in a reduction of the scatter fraction to the level of $\sim 35\%$ ⁴⁴. As regards the selection efficiency for the prompt photon with energy of 1160 keV which in both cases (LYSO and plastic) is registered predominantly via Compton effect (in $\sim 100\%$ for plastics and 89% for LYSO) the selection efficiency ϵ_{sel-p} (both for LYSO and plastic scintillators) was equal to 0.66, just as a fraction of the energy deposition spectrum with deposited energy larger than the one from the 511 keV photons.

The above quoted values of attenuation coefficients and the fractions of photoelectric and Compton effects were extracted from the data base maintained by the National Institute of Standards and Technology⁴⁵.

2.2 Detailed Monte Carlo simulations

The detailed studies of the spatial and time resolution of the mean lifetime positronium images as a function of the time resolution of the detector system were performed on the example of the cost effective total-body PET built from plastic scintillators. Analogously as in reference¹ the ideal J-PET detector system consisting of four concentric cylindrical layers, filled with plastic scintillator strips, was simulated. The inner radius and axial field-of-view were chosen to be $R = 43$ cm and $AFOV = 200$ cm, respectively. For the single plastic strip, the cross section of 7×19 mm² is chosen as it is used in the current version of the J-PET prototype⁴⁶.

In the plane comprising the central detector axis the 1-mm radius cylindrical ⁴⁴Sc sources surrounded with different materials were simulated. Their positions were chosen according to the NEMA NU 2-2012 norm⁴⁷, and for each position a different mean lifetime of ortho-positronium was assumed, as it is listed in the Table 1. The values of the mean ortho-positronium lifetime were chosen in the range expected for ortho-positronium produced in the human body^{1,5}.

Table 1: Coordinates of simulated point-like sources positioned according to the NEMA norm. Each source is characterized by a different mean lifetime of ortho-positronium.

Position	Coordinates [cm]	Simulated oPs mean lifetime [ns]
1	(1, 0, 0)	2.0
2	(10, 0, 0)	2.4
3	(20, 0, 0)	2.8
4	(1, 0, 75)	2.2
5	(10, 0, 75)	2.6
6	(20, 0, 75)	3.0

For the studies presented in this article 5×10^6 events with the emission of prompt gamma from ⁴⁴Sc decay followed by the creation of ortho-positronium and its subsequent decay into two photons were generated. Subsequently, for each generated event, the response of the idealized J-PET scanner was simulated and then the standard 2γ image as well as the mean lifetime positronium image were reconstructed. Standard PET image showing the density distribution of annihilation points was performed using TOF filtered back projection method (TOF-FBP)⁴⁸ and the mean lifetime positronium image is reconstructed by the determination of the annihilation point and ortho-positronium lifetime on the event by event basis. Positronium lifetime image is constituted from mean ortho-positronium lifetimes determined for each image voxel.

The simulations were conducted in the following steps: For each event (i) the position of the annihilation was generated, in the arrangement required by the NEMA⁴⁷ norm (Table 1); (ii) the prompt photon with energy of 1160 keV was emitted isotropically; (iii) in each event a creation of ortho-positronium atom was assumed and its decay time was generated with the exponential probability density distribution assuming mean lifetime depending on the position (see Table 1); (iv) for

each event an ortho-positronium annihilation (pick-off or conversion processes) into two 511 keV back-to-back photons was generated assuming the isotropic emission independent of the emission of the prompt gamma; (v) hit-positions and energy depositions of annihilation photons and prompt gamma in the J-PET scanner were simulated taking into account cross sections for Compton interactions of gamma photons in plastic scintillators; (vi) the experimental hit-position resolutions (axial and radial) was accounted for by smearing the generated positions with Gaussian functions having 5 mm (FWHM) as expected for J-PET scanner with the assumed SiPM and WLS readout^{1,44}; (vii) the time resolution was included by smearing the generated interaction times with Gaussian distributions corresponding to CRT values of {140, 50, 10} ps (the values after smearing will be referred to as *registered*); (viii) for each *registered* event, the time and position of annihilation point as well as the time of the emission of prompt gamma was reconstructed; and finally (ix) for each voxel of the image a mean ortho-positronium lifetime was reconstructed.

The simulation methods for the above listed steps were described in details in the previous publications^{1,26,43,49,50}.

3 Results

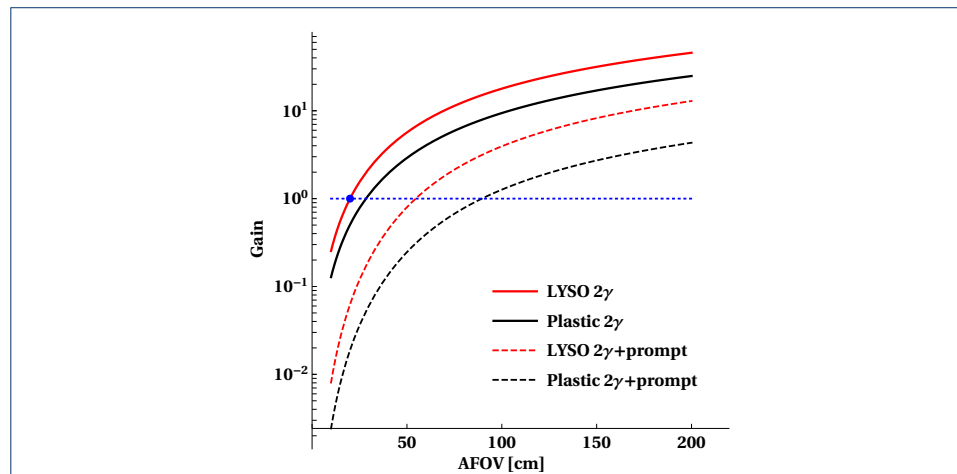


Figure 3: Relative gain in sensitivity S as a function of the AFOV of the scanner. The gain is calculated relative to sensitivity for the standard 2γ imaging using LYSO PET with AFOV = 20 cm (blue dot). The gains for 2γ (solid lines) as well as for $2\gamma + \gamma_{prompt}$ (dashed lines) are shown for LYSO and plastic scintillators as indicated in the legend. The red and black colour indicate result for the LYSO and plastic scintillators, respectively.

Figure 3 presents the gain of the sensitivity calculated as defined by (Eq. 1) in section 2. The gain is calculated with respect to the sensitivity of the PET from LYSO crystals with AFOV = 20 cm for the standard 2γ imaging (indicated as blue dot in the figure). The relative gain is presented as a function of AFOV of the scanner. Dashed lines indicate that for the $(2\gamma + \gamma_{prompt})$ triple coincidences with AFOV = 200 cm the achievable gain is equal to factor of about 12.2 and 4.7 for LYSO and plastic based PET, respectively. It indicates that the $2\gamma + \gamma_{prompt}$ positronium

imaging is feasible with the total-body PET scanners with sensitivities even higher than the one of the current PET with AFOV ~ 20 cm. For the comparison, in order to cross-check the estimations, the gain for the standard 2γ imaging is shown. The red and black solid lines indicate sensitivity gain expected for the registration of the image forming events with two back-to-back annihilation photons (2γ) calculated for the LYSO and plastic based scanners, respectively. As expected,^{51,52} for the whole body scan with total-body LYSO PET the sensitivity is increased by more than factor of forty. The black solid line indicates that for the whole-body scan, the total-body PET from plastic scintillators also provides a large, about twentyfold, gain in sensitivity.

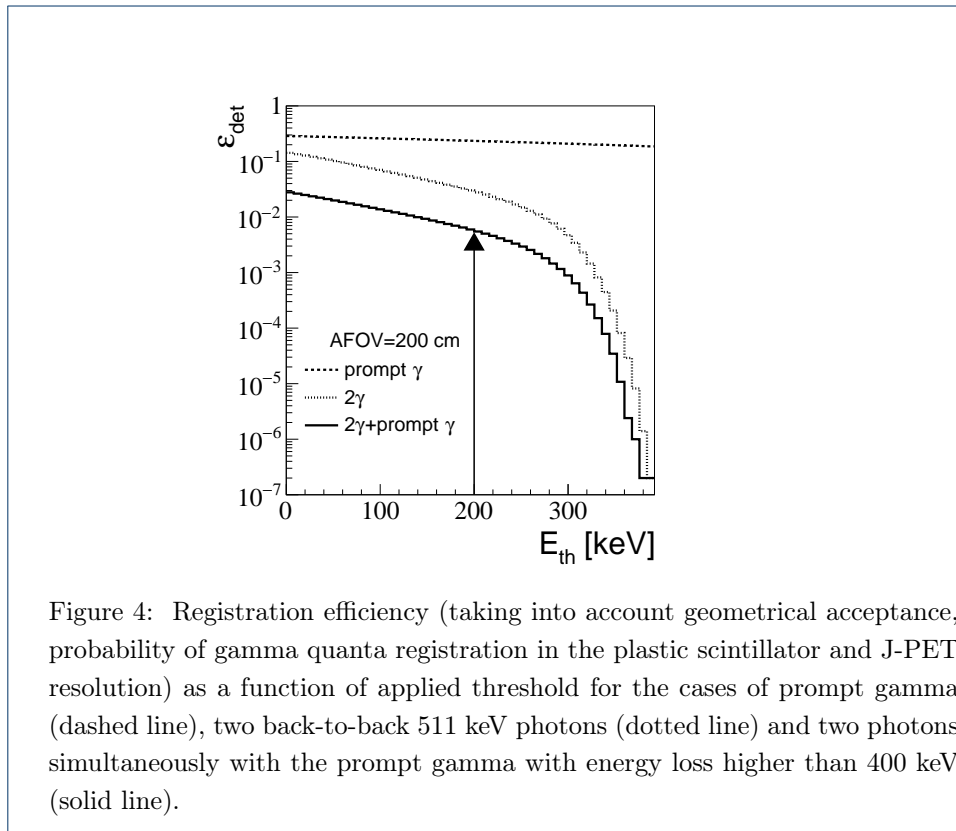


Figure 4 presents sensitivities (detection efficiency) calculated using detailed Monte-Carlo method (section 2) for the case of the total-body plastic PET with AFOV = 200 cm and total plastic thickness of 6 cm. The dashed line indicates overall geometrical and detection efficiency for the registration of the prompt gamma (1160 keV) and the dotted histogram shows detection efficiency for the registration of the back-to-back 511 keV photons. The results are shown as a function of the energy deposition threshold. Solid line indicates overall efficiency for the registration of back-to-back photons with coincident detection of prompt photon with energy deposition larger than 400 keV. Such condition enables to disentangle prompt gamma from 511 keV photons. In order to decrease the scatter fraction down to 35% a minimum energy deposition of 200 keV is required for the 511 keV photons^{44,50,53}. Therefore, for the 2γ positronium mean lifetime imaging of the 200 cm long objects,

with the plastic total-body PET, a total detection and selection efficiency of about 0.5% is expected (as indicated in Fig 4 by an arrow). Thus with the plastic total-body PET about $6.6 \cdot 10^8$ image forming triple coincidence events ($2\gamma + \gamma_{prompt}$) may be collected assuming (i) 20 min scan according to the standard whole-body protocol, (ii) activity of 370 MBq (10 mCi) administered to the patient⁵², (iii) detection sensitivity of 0.5%, and (iv) 30% fraction of positron annihilations through the formation of ortho-positronium atoms in the body. This corresponds to about 10^4 event forming events per cubic centimeter for the plastic based total-body PET. While, when taking into account ratio between dashed lines in Fig. 3, $2.6 \cdot 10^4$ events per cubic centimeter are expected for LYSO based total-body PET. These numbers will be used later on to estimate mean lifetime resolution for positronium imaging.

Fig. 5 compares standard PET images determined for the point-like sources arranged according to the NEMA norm recommendations (Tab. 1). The coronal XZ cross-section along $y = 0$ cm are shown. Left column shows images obtained directly as a density distribution of annihilation points assuming TOF resolution of CRT = 10 ps (top row), CRT = 50 ps (middle row), and CRT = 140 ps (bottom row). Middle column indicates images determined using the TOF filtered back projection (TOF-FBP) algorithm, and right column presents enhanced view of images of the source close to the centre of the scanner. The obtained point spread functions (PSF) are listed in Tab. 2. The result indicates that already for CRT = 50 ps the PSF of the direct image is comparable with the PSF achievable when applying reconstruction with TOF-FBP algorithm.

Finally the results for the mean lifetime positronium image are presented. The triple coincidence events ($2\gamma + \gamma_{prompt}$) were simulated and analyzed as it is described in section 2. When using events with triple coincidences $2\gamma + \gamma_{prompt}$ it is possible to reconstruct position and time of the creation of two back-to-back photons and the time of the creation of the positron. The latter can be deduced based on the time and position of interaction of the prompt gamma and the position of the annihilation point. Thus for each voxel of the image a spectrum of differences between the time of annihilation and the time of positron emission can be created enabling mean lifetime ortho-positronium reconstruction. Fig. 6 compares ortho-positronium mean lifetimes images reconstructed based on simulated signals (described in section 2) to the generated image. The simulation and reconstruction was performed for three cases assuming time resolution of the scanner to be CRT = 10 ps, 50 ps and 140 ps. All reconstructed images reflect the generated image very well. The quantitative comparison is shown in the left panel of Fig. 7. Figure shows that for each simulated source position, the reconstructed mean lifetimes agree with the generated values within about 10 ps. The resolution of the reconstructed mean lifetime depends on (i) the detector's time and spatial resolution, (ii) on the mean ortho-positronium lifetime (τ_{tissue}), as well as (iii) on the number of events assigned to a given voxel. The right panel of Fig. 7 presents the resolution as a function of the number of events. The result indicates that a resolution of better than 20 ps (RMS) is achievable for the number of image forming events (10^4) expected per cubic centimeter in a 20 minutes total-body scan. The result is valid for all tested CRT values since they are more than order of magnitude smaller than the mean lifetime of ortho-positronium atoms in the body (few nanoseconds), and

therefore the reconstruction resolution of the mean lifetime depends predominantly on τ_{tissue} and may be approximately estimated as τ_{tissue}/\sqrt{N} , where N denotes number of events in a given voxel. It is important to stress that in Fig 4 the values of sensitivities do not include losses in the number of events due to attenuation and scattering of photons in the patient. Inclusion of attenuation would decrease the number of positronium-image forming events by about an order of magnitude. Therefore, at the present early stage of the development of this method it would be appropriate to strive to achieve first experimental images with larger voxel's size (e.g. $2 \times 2 \times 2 \text{ cm}^3$) ensuring the statistics of (10^4) events per voxel.

CRT [ps]	PSF direct image [mm]		PSF TOF-FBP image [mm]	
	radial	axial	radial	axial
10	4.2	4.8	4.5	5.5
50	5.4	5.2	4.5	5.5
140	10.2	6.8	5.0	6.0

Table 2: Point Spread Function (PSF) obtained for the direct and TOF-FBP images as a function of CRT. Values presented are for position ($x = 20, y = 0, z = 75$) cm.

4 Discussion

Recently it was reported that the mean lifetime of ortho-positronium, which is copiously produced in the body during the PET investigation, may be used as the in-vivo diagnostic indicator complementary to the currently available SUV index^{1,3}. In this article we assess the feasibility of ortho-positronium mean lifetime imaging using 2γ decays which occurs in the tissue due to the pick-off and ortho- to para-positronium conversion processes. We have shown that with the advent of the total-body PET and the improvement of time resolution to tens of picoseconds the 2γ ortho-positronium mean lifetime imaging may be performed with the sensitivity and spatial resolution comparable with the current standard 2γ metabolic imaging obtainable by PET scanners with AFOV of about 20 cm. We also have shown that having time resolution of tens of picoseconds the 2γ mean lifetime positronium imaging becomes feasible for the cost effective total-body J-PET scanner built from plastic scintillators. Calculations were performed taking into account ^{44}Sc labeled radiopharmaceutical emitting prompt gamma with the energy of 1160 keV. In the calculations of the sensitivity gain the attenuation of both two 511 keV annihilation and prompt photons in the 20 cm diameter water phantom were taken into account. Quantitative estimations show that for the whole-body scan, the overall sensitivity for registration and image forming selection of $2\gamma + \gamma_{prompt}$ events exceeds the sensitivity of current PET 2γ metabolic imaging twelvefold in case of total-body PET based on LYSO scintillators and fourfold in case of the total-body PET from plastic scintillators. Moreover, the obtained result (Fig. 3) indicates that the sensitivity for ortho-positronium mean lifetime image is becoming comparable with current PET sensitivities for AFOV of about 56 cm (LYSO PET) and 87 cm (plastic PET). Finally the mean lifetime resolution achievable with the presented method for total-body PET is ranging between 10 ps and 20 ps for LYSO and plastic PET systems and it is predominantly due to the large (few ns) ortho-positronium mean lifetime



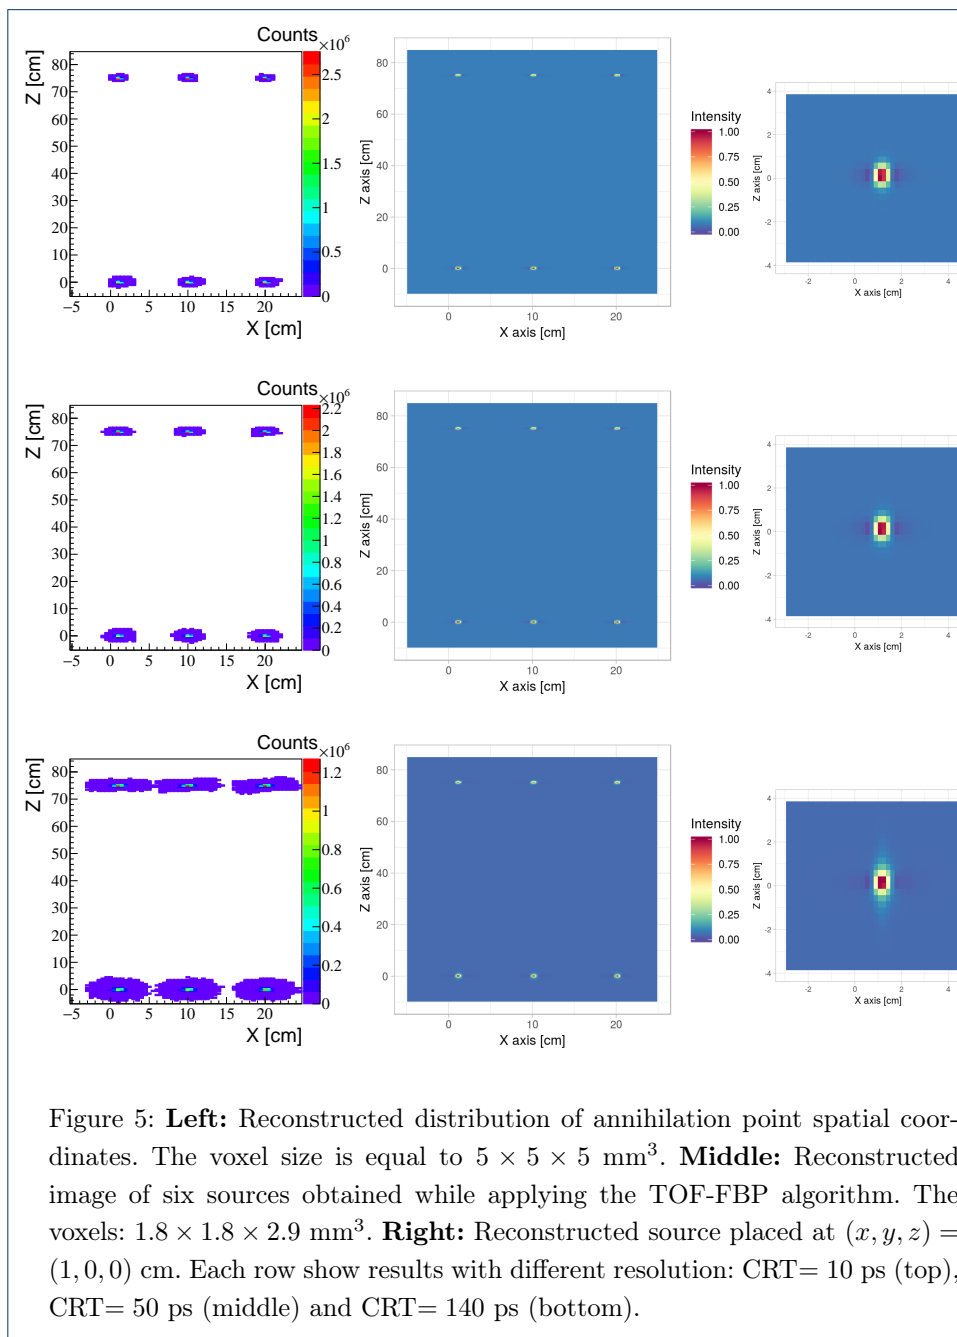


Figure 5: **Left:** Reconstructed distribution of annihilation point spatial coordinates. The voxel size is equal to $5 \times 5 \times 5$ mm³. **Middle:** Reconstructed image of six sources obtained while applying the TOF-FBP algorithm. The voxels: $1.8 \times 1.8 \times 2.9$ mm³. **Right:** Reconstructed source placed at $(x, y, z) = (1, 0, 0)$ cm. Each row show results with different resolution: CRT= 10 ps (top), CRT= 50 ps (middle) and CRT= 140 ps (bottom).

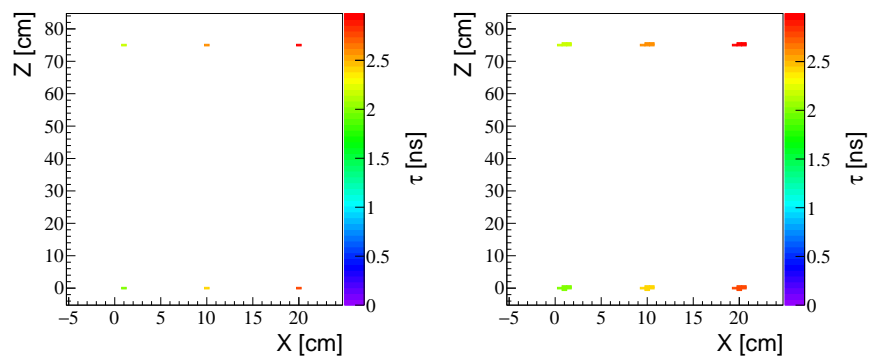

(a) Generated positronium lifetime distribution.


(b) Reconstructed positronium lifetime distribution (CRT=10 ps).

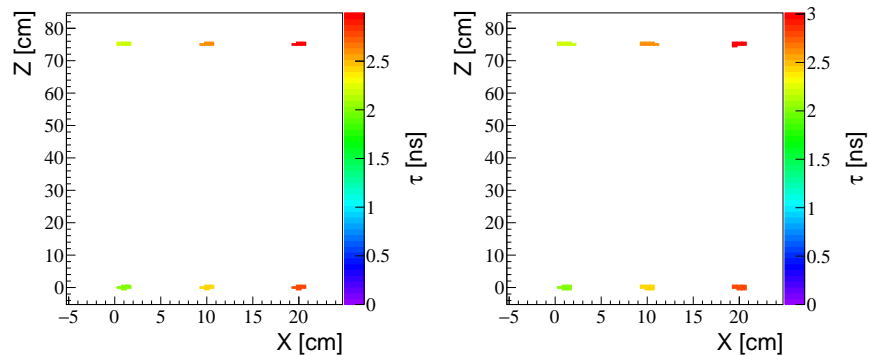

(c) Reconstructed positronium lifetime distribution (CRT=50 ps).

(d) Reconstructed positronium lifetime distribution (CRT=140 ps).

Figure 6: Distributions of generated positronium lifetimes (a), and reconstructed ones, assuming the CRT value of 10 ps (b), 50 ps (c) and 140 ps (d). The voxel size is equal to $5 \times 5 \times 5 \text{ mm}^3$.

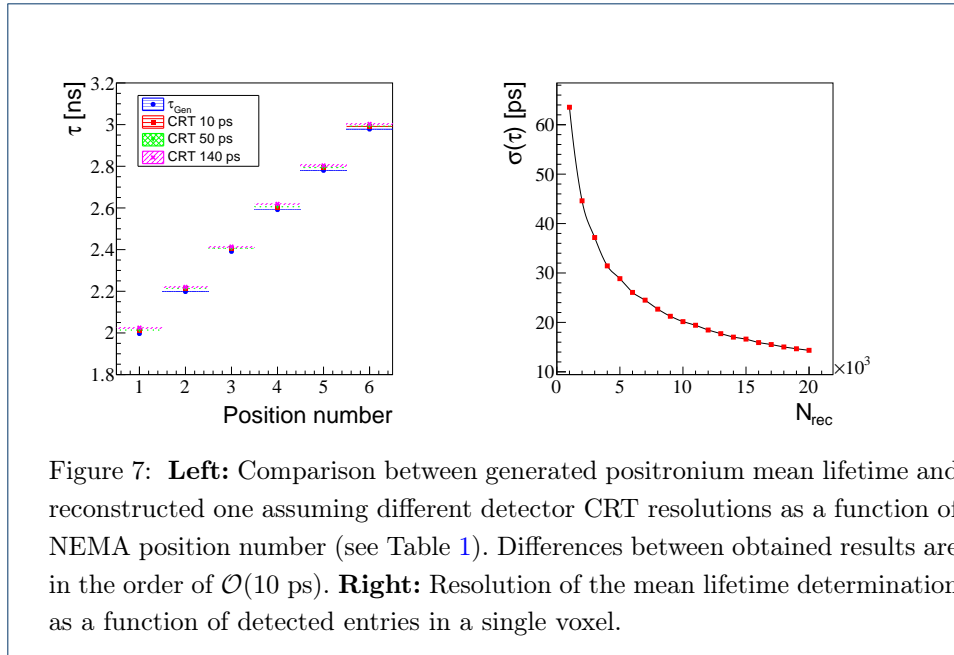

while it is fairly independent of the more than order of magnitude smaller CRT values.

Positronium mean lifetime imaging with two photons, discussed in this article, is beneficial in relation to imaging using three photons due to the smaller attenuation of photons in the body and higher detection sensitivity. In case of the ortho-positronium 2γ imaging the attenuation of photons in the body will be much smaller than for the $oPs \rightarrow 3\gamma$ imaging. This is because in the latter case there is one more photon which needs to escape from the body and the energy of photons in case of $oPs \rightarrow 3\gamma$ ranges from 0 to 511 keV and thus these photons having energy lower than 511 keV are on the average more strongly absorbed in the body with respect to 511 keV photons from the 2γ annihilations. Moreover, the ortho-positronium mean lifetime imaging based on the $oPs \rightarrow 2\gamma$ events may directly be applied in the present TOF-PET systems. Making the application of the proposed method realistic in the near future.

5 Conclusions

The method discussed in this article, in general enables to determine a spectrum of positron lifetime on a voxel by voxel basis. Allowing to determine not only an image of the mean lifetime of ortho-positronium (or in general a distribution of mean ortho-positronium lifetimes³⁸), but it also gives access to the images of mean lifetime of the direct electron-positron annihilations and the probability of the positronium formation⁴. Establishing correlations of these parameters with the cancer grade requires systematic long-term study. There are first in-vitro measurements indicating differences in positronium properties in healthy and cancerous tissues⁵. The application of the method advocated in this article makes an in-vivo investigations possible which, due to the fact that positronium interacts in the living organisms with bio-active molecules, may reveal yet unknown features useful for diagnosis.

Finally it is worth noting that one of the important feature of the mean ortho-positronium lifetime image is that it does not require attenuation corrections⁴. This is because of the lifetime of ortho-positronium is independent of photons attenuation, and though suppression of photons in the body affects the statistics in a given voxel, it does not affect the shape of the lifetime spectrum, leaving the mean lifetime unaltered.

Ethics approval and consent to participate

Not applicable

Consent for publication

Not applicable

Availability of data and material

The data that support the findings of this study are available from the corresponding author upon request.

Competing interests

The authors declare that they have no competing interests

Funding

This work was supported by The Polish National Center for Research and Development through grant INNOTECH-K1/INI/64/159174/NCBR/12, the Foundation for Polish Science through the MPD and TEAM POIR.04.04.00-00-4204/17 programmes, the National Science Centre of Poland through grants no. 2016/21/B/ST2/01222, 2017/25/N/NZ1/00861, the Ministry for Science and Higher Education through grants no. 6673/IA/SP/2016, 7150/E-338/SPUB/2017/1 and 7150/E-338/M/2017, 7150/E-338/M/2018 and the Austrian Science Fund FWF-P26783.

Authors' contributions

All authors contributed to the manuscript discussion, interpretation of results, correction and approval and elaboration of the simulation, analysis and reconstruction methods used to achieve the described result. PM has conceived the method, derived the analytic estimation of sensitivity, and was a major contributor in writing the manuscript. DK prepared the Monte Carlo simulations and analyzed positronium mean lifetime distributions. RS provided reconstruction with TOF-FBP algorithm.

Acknowledgements

The authors acknowledge technical and administrative support of A. Heczko, M. Kajetanowicz and W. Migdał.

Author details

¹Faculty of Physics, Astronomy and Applied Computer Science, Jagiellonian University, prof. Stanisława Łojasiewicza 11, 30-348 Cracow, Poland. ²INFN, Laboratori Nazionali di Frascati, 00044 Frascati, Italy. ³Institute of Nuclear Physics PAN, Cracow, Poland. ⁴Institute of Physics, Maria Curie-Skłodowska University, 20-031 Lublin, Poland. ⁵Faculty of Physics, University of Vienna, 1090 Vienna, Austria. ⁶Department of Complex Systems, National Centre for Nuclear Research, 05-400 Otwock-Świerk, Poland. ⁷High Energy Physics Division, National Centre for Nuclear Research, 05-400 Otwock-Świerk, Poland. ⁸2nd Department of General Surgery, Jagiellonian University Medical College, Cracow, Poland. ⁹Department of Physics, College of Education for Pure Sciences, University of Mosul, Mosul, Iraq. ¹⁰Department of Electronics and Information Systems, MEDISIP, Ghent University-IBiTech, De Pintelaan 185 block B, B-9000 Ghent, Belgium.

References

- Moskal P, et al. Feasibility study of the positronium imaging with the J-PET tomograph. *Phys Med Biol*. 2019 mar;64(5):055017. Available from: <https://doi.org/10.1088/2F1361-6560/2Faaf20>.
- Harpen MD. Positronium: Review of symmetry, conserved quantities and decay for the radiological physicist. *Medical Physics*. 2004;31(1):57–61. Available from: <http://dx.doi.org/10.1118/1.1630494>.
- Moskal P, Jasińska B, Stępień E, Bass S. Positronium in Medicine and Biology. *Nature Reviews Physics*. 2019;1:527–529. Available from: <https://doi.org/10.1038/s42254-019-0078-7>.
- Moskal P, et al.. TOF-PET tomograph and a method of imaging using a TOF-PET tomograph, based on a probability of production and lifetime of a positronium;. Patent US 9851456 (2017), PL 227658 (2013).
- Jasińska B, et al. Human Tissues Investigation Using PALS Technique. *Acta Phys Polon*. 2017;B48:1737.
- Jasińska B, et al. Human Tissue Investigations Using PALS Technique — Free Radicals Influence. *Acta Phys Polon*. 2017;A132:1556.
- Pietrzak R, Borbulak S, Szatanik R. Influence of neoplastic therapy on the investigated blood using positron annihilation lifetime spectroscopy. *Nukleonika*. 2013;58:199–202.
- Hugenschmidt C, Ceeh H. The free volume in dried and H₂O-loaded biopolymers studied by positron annihilation measurements. *J Phys Chem*. 2014;B118:9356.
- Reisfeld R, et al. Porous glasses as a host of luminescent materials, their applications and sites elective determination. *Journal of luminescence*. 2016;169:440–444.
- Chen H, et al. Free-Volume Depth Profile of Polymeric Membranes Studied by Positron Annihilation Spectroscopy: Layer Structure from Interfacial Polymerization. *Macromolecules*. 2007;40(21):7542–7557.
- Gajos A, et al. Trilateration-based reconstruction of ortho-positronium decays into three photons with the J-PET detector. *Nucl Instrum Meth*. 2016;A819:54–59.

12. Gajos A. Investigations of fundamental symmetries with the electron-positron systems. Jagiellonian University; 2018.
13. Szkliniarz K, et al. Medical Radioisotopes Produced Using the Alpha Particle Beam from the Warsaw Heavy Ion Cyclotron. *Acta Phys Polon.* 2015;A127:1471.
14. Sitarz M, Cussonneau JP, Matulewicz T, Haddad F. Radionuclide candidates for $\beta + \gamma$ coincidence PET: An overview. *Applied Radiation and Isotopes.* 2020;155:108898. Available from: <http://www.sciencedirect.com/science/article/pii/S096980431930418X>.
15. Garwin RL. Thermalization of Positrons in Metals. *Phys Rev.* 1953 Sep;91:1571–1572. Available from: <https://link.aps.org/doi/10.1103/PhysRev.91.1571>.
16. Consolati G, Quasso F. Positronium–oxygen interactions in polytrimethylsilylpropine membranes. *Appl Phys.* 1998;B66:371–376.
17. Ferrell RA. Ortho-para positronium quenching by paramagnetic molecules and ions. *Phys Rev.* 1958;110:1355–1357.
18. Zgardzińska B, Białko W, Jasińska B. Ortho-para spin conversion of Ps by paramagnetic O₂ dissolved in organic compounds. *Nukleonika.* 2015;60(4):801–804.
19. Jasińska B, Moskal P. A new PET diagnostic indicator based on the ratio of 3 γ /2 γ positron annihilation. *Acta Phys Polon.* 2017;B48:1577.
20. van Sluis J, et al. Performance Characteristics of the Digital Biograph Vision PET/CT System. *J Nucl Med.* 2019 Jan;60(7):1031.
21. Nemallapudi MV, Gundacker S, Lecoq P, Auffray E, Ferri A, Gola, et al. Sub-100 ps coincidence time resolution for positron emission tomography with LSO:Ce codoped with Ca. *Phys Med Biol.* 2015;60(12):4635. Available from: <http://stacks.iop.org/0031-9155/60/i=12/a=4635>.
22. Bisogni M, Guerra AD, Belcari N. Medical applications of silicon photomultipliers. *Nuclear Inst and Methods in Physics Research.* 2019;A926:118–128.
23. Gundacker S, et al. High-frequency SiPM readout advances measured coincidence time resolution limits in TOF-PET. *Phys Med Biol.* 2019;64(5):055012.
24. Bieniosek MF, Cates JW, Grant AM, Levin CS. Analog filtering methods improve leading edge timing performance of multiplexed SiPMs. *Phys Med Biol.* 2016 aug;61(16):N427–N440. Available from: <https://doi.org/10.1088/2F0031-9155/2F61/2F16/2Fn427>.
25. Seifert S, van Dam HT, Schaart DR. The lower bound on the timing resolution of scintillation detectors. *Phys Med Biol.* 2012 03;57:1797–814.
26. Moskal P, et al. Time resolution of the plastic scintillator strips with matrix photomultiplier readout for J-PET tomograph. *Phys Med Biol.* 2016;61:2025.
27. Berg E, Cherry SR. Using convolutional neural networks to estimate time-of-flight from PET detector waveforms. *Phys Med Biol.* 2018;63(2):02LT01.
28. Kim K, et al. Analog and digital signal processing method using multi-time-over-threshold and FPGA for PET. *Medical Physics.* 2018;45(9):4104–4111.
29. Pałka M, et al. Multichannel FPGA based MVT system for high precision time (20 ps RMS) and charge measurement. *JINST.* 2017;12(08):P08001.
30. Zhu B, et al. Image reconstruction by domain-transform manifold learning. *Nature.* 2018;555:487–492.
31. Ota R, et al. Coincidence time resolution of 30 ps FWHM using a pair of Cherenkov-radiator-integrated MCP-PMTs. *Phys Med Biol.* 2019 mar;64(7):07LT01. Available from: <https://doi.org/10.1088/2F1361-6560/2F64/7/07LT01>.
32. Lecoq P. Pushing the Limits in Time-of-Flight PET Imaging. *IEEE Transactions on Radiation and Plasma Medical Sciences.* 2017;1(6):473–485.
33. Nolet F, et al. Quenching Circuit and SPAD Integrated in CMOS 65 nm with 7.8 ps FWHM Single Photon Timing Resolution. *Instruments.* 2018;2(4). Available from: <https://www.mdpi.com/2410-390X/2/4/19>.
34. Nolet F, et al. Digital SiPM channel integrated in CMOS 65 nm with 17.5 ps FWHM single photon timing resolution. *Nucl Instr Meth Phys Res.* 2018;A912:29 – 32. Available from: <http://www.sciencedirect.com/science/article/pii/S0168900217310720>.
35. Badawi RD, et al. First Human Imaging Studies with the EXPLORER Total-Body PET Scanner. *J Nucl Med.* 2019;60:299–303.
36. Surti S, Karp JS. Impact of event positioning algorithm on performance of a whole-body PET scanner using one-to-one coupled detectors. *Phys Med Biol.* 2018 mar;63(5):055008. Available from: <https://doi.org/10.1088/2F1361-6560/2F63/5/055008>.
37. National Nuclear Data Center; 2016. Accessed: 20.01.2016. <http://www.nndc.bnl.gov/>.
38. Dulski K, et al. Analysis Procedure of the Positronium Lifetime Spectra for the J-PET Detector. *Acta Phys Pol.* 2017;A132:1637.
39. Champion C. Moving from organ dose to microdosimetry: contribution of the Monte Carlo simulations. *Brazilian Archives of Biology and Technology.* 2005 10;48:191 – 199.
40. NUCLEIDE-LARA - Library for alpha, X and gamma emissions; 2017. Accessed: 10.02.2018. <http://www.nucleide.org/NucData.htm>.
41. Leung EK, Judenhofer MS, Cherry SR, Badawi RD. Performance assessment of a software-based coincidence processor for the EXPLORER total-body PET scanner. *Phys Med Biol.* 2018 sep;63(18):18NT01. Available from: <https://doi.org/10.1088/2F1361-6560/2F63/18/18NT01>.
42. Moskal P, et al. The NEMA characteristics of the modular total-body J-PET tomograph. in print. 2019;.
43. Moskal P, et al. Test of a single module of the J-PET scanner based on plastic scintillators. *Nucl Instrum Meth.* 2014;A764:317–321.
44. Kowalski P, et al. Estimating the NEMA characteristics of the J-PET tomograph using the GATE package. *Phys Med Biol.* 2018;63:165008.
45. National Institute of Standards and Technology; 2019. Accessed: 10.02.2019. <https://www.nist.gov/pml>.

46. Niedźwiecki S, et al. J-PET: a new technology for the whole-body PET imaging. *Acta Phys Polon.* 2017;B48:1567.
47. NEMA. Performance measurements of positron emission tomographs; 2012. National Electrical Manufacturers Association (NEMA NU 2-2012).
48. Conti M, et al. First experimental results of time-of-flight reconstruction on an LSO PET scanner. *Phys Med Biol.* 2005 sep;50(19):4507–4526. Available from: <https://doi.org/10.1088/0031-9155/50/19/2F006>.
49. Kamińska D, et al. A feasibility study of ortho-positronium decays measurement with the J-PET scanner based on plastic scintillators. *Eur Phys J.* 2016;C76(8):445.
50. Moskal P, et al. A novel method for the line-of-response and time-of-flight reconstruction in TOF-PET detectors based on a library of synchronized model signals. *Nucl Instrum Meth.* 2015;A775:54–62.
51. Cherry SR, et al. Total-body imaging: Transforming the role of positron emission tomography. *Science Translational Medicine.* 2017;9:381.
52. Cherry SR, et al. Total-body PET: maximizing sensitivity to create new opportunities for clinical research and patient care. *Journal of Nuclear Medicine.* 2017;59:3–12.
53. Kowalski P, et al. Scatter Fraction of the J-PET Tomography Scanner. *Acta Phys Polon.* 2016;B47:549.