

Compressive Raman microspectroscopy parallelized by single-photon avalanche diode arrays

Clémence Gentner¹ [†], Samuel Burri² [†], Edoardo Charbon² [⊗], Claudio Bruschini² [⊗], Hilton B. de Aguiar¹ 

¹Laboratoire Kastler Brossel, ENS-Université PSL, CNRS, Sorbonne Université, Collège de France, 24 rue Lhomond, 75005 Paris, France; ²Advanced Quantum Architecture Lab (AQUA), EPFL, 2002 Neuchâtel, Switzerland

Abstract

We demonstrate an efficient and scalable compressive Raman parallelization scheme based on single-photon avalanche diode (SPAD) arrays to reach pixel dwell times of 23 μ s, representing over 10x speed-up using the otherwise weak spontaneous Raman effect.

 **For correspondence:**
claudio.bruschini@epfl.ch,
h.aguiar@lkb.ens.fr
www.lkb.upmc.fr/opticalimaging/
www.epfl.ch/labs/aqua/

[†]These authors contributed equally to the work.

Funding: This work was supported by the Emergence program from Sorbonne University (FANCIER).

Compressive Raman has enabled high-speed spectral imaging by compressing the hyperspectrum at its acquisition stage, exploiting data sparsity (Wilcox et al., 2013; Cebeci, Mankani, and Ben-Amotz, 2018; Lin and De Aguiar, 2021). The hardware of this emerging technology relies on a programmable spectrometer based on a spatial light modulator coupled to a single-pixel detector (instead of the more costly and read-out noise limited charge-coupled devices). While acquisition and processing times are already considerably reduced compared to conventional Raman imaging, further speed gains could in principle be achieved by increasing the excitation power (at constant energy). Nevertheless, such an approach would be fundamentally limited by the detector's dead time. For instance, if one detects 10 photons (Wilcox et al., 2013), current commercially available single-pixel SPADs would reach pixel dwell times τ_{pdt} at best 1 μ s. Hence, spatial detection parallelization with high-throughput low-noise sensors constitutes the operating lever to reach real-time imaging.

While SPAD arrays are being developed at a fast pace (Bruschini et al., 2019), they were until now incompatible with the requirements needed for high-speed imaging with the weak spontaneous Raman effect. Here, we introduce a novel compressive Raman spectrometer layout equipped with a new high-throughput SPAD linear array, LinoSPAD2 (Lubin et al., 2021), to heavily parallelize the single-pixel approach. In addition to data compression in the spectral domain, this architecture allows spatial multiplexing with line scan illumination, leading to acquisition speeds only fundamentally limited by either inertial motion of 1D scanners or the detector's dead time. In this initial demonstration, an effective $\tau_{pdt} = 23 \mu$ s was achieved with the spontaneous Raman effect, with potential to reduce this twenty-fold, thus paving the way for video-rate imaging in spontaneous Raman microspectroscopy.

In programmable spectrometers for compressive Raman, the emitted light from the point-scanned sample is steered into a conventional Czerny-Turner spectrometer (Wilcox et al., 2012;

Wilcox et al., 2013; Sturm et al., 2019; Soldevila et al., 2019; Corden et al., 2018; Rehrauer et al., 2018; Scotté et al., 2019; Scotté et al., 2020). The camera is replaced by a digital micromirror device (DMD) which sends specific spectral bins, selected according to the chemical identification algorithm used (Wilcox et al., 2012; Réfrégier et al., 2018; Soldevila et al., 2019), towards a single-pixel SPAD. Spatial parallelization of this scheme (see Fig. 1) speeds up the acquisition by $N_{\text{SPAD}} \frac{PDE_{\text{array}}}{PDE_{\text{sp}}}$, where N_{SPAD} is the number of spatial pixels and PDE is the SPAD photon detection efficiency (either single-pixel (SP) or array). The LinoSPAD2 linear array is composed of 512 low-noise and high-sensitivity pixels implemented in 180 nm standard CMOS technology, with 1:1 direct read-out by a pair of custom FPGA boards (Burri, Bruschini, and Charbon, 2017). This enables full reconfigurability of the photon counting and/or time-stamping functions.

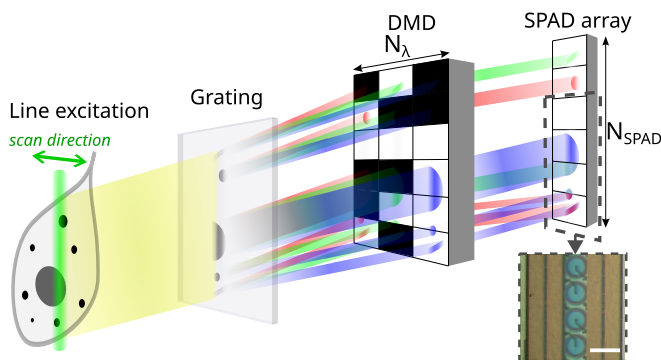


Figure 1. Parallelized compressive Raman microspectroscopy. The line-shaped laser light is focused on the sample and imaged onto the grating of the spectrometer, defining the N_{λ} wavelength bins on the DMD. The dimension along the excitation line on the DMD parallelizes the detection of N_{SPAD} spatial pixels. Black DMD pixels represent discarded wavelength bins. An image is formed by scanning the line in its orthogonal direction. Inset: brightfield image of four pixels of the LinoSPAD2 array. Scale bar: 30 μm .

One of the challenges in implementing this parallelization scheme is due to the DMD's own dispersion. Indeed, a DMD is a grating whose dispersion increases the sensitivity to alignment of the quality of the spectrometer PSF, giving rise to crosstalk between the SPAD pixels when moving away from the optimal wavelength (see Fig. 2 thumbnails). This effect led to the widespread adoption of large-area single-pixel detectors (typically photomultipliers). Previously, we have described a methodology to overcome this issue and better control the dispersion in a programmable spectrometer using a 190 μm -wide single-pixel SPAD (Sturm et al., 2019). We now reach PSFs down to tens of μm , a typical size of SPADs in arrays, effectively enhancing the bandwidth coupling for a given spectral range, in this case the stretch resonances (C-H, O-H) spectral range (Fig. 2, bottom). Furthermore, the PSF undergoes a displacement mainly along the SPAD array direction and is stable enough over the spectral range, hence minimizing inter-pixel spectral coupling (Fig. 2, middle).

We demonstrate parallelized high-speed chemical imaging. Instead of 2D point scanning, the sample is excited by a laser line (Spectra Physics, Millennia eV10S, $\lambda=532$ nm) that is 1D scanned (Thorlabs GVS012) using an objective (20 \times , NA 0.5, Nikon) to focus the line to a length of 90 μm . The epi-detected Raman signal from the line excitation is descanned and steered into the spectrometer coupled with the SPAD array through a 1D confocal layout using a 30 μm slit at the entrance plane. The energy densities used were 4 and 40 $\mu\text{J} \mu\text{m}^{-2}$ for effective $\tau_{\text{pdt}} = 23$ and 230 μs , respectively. We demonstrate the speed advantage using established supervised compressive Raman methods (Réfrégier et al., 2018) and as a sample, polystyrene (PS) and polymethylmethacrylate (PMMA) beads of 6 and 5 μm diameters, respectively, on top of a coverslip covered with water (spectra shown in Fig. 2, bottom). Fig. 3 shows a 3D chemical image (x, y, z) composed of 128 \times 531 \times 40 pixels. A standard denoising scheme was performed using Fourier domain Gaussian smoothing. Each (x, y) slice (Fig. 3, inset) was acquired by horizontally scanning at 10 and 1 ms line dwell time τ_{ldt} , orders of magnitude faster than conventional cameras in non-compressed approaches due

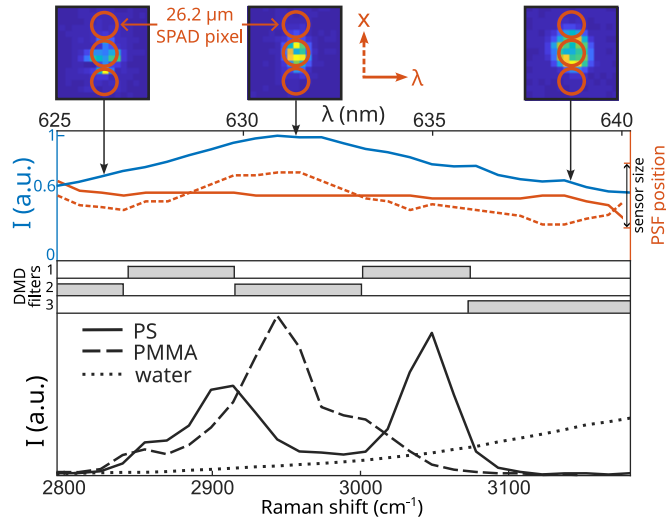


Figure 2. Characterization of the programmable spectrometer. (Top panel) Available spectral detection efficiency (blue) is limited by SPAD pixel crosstalk (see thumbnails for images acquired at the SPAD plane with an auxiliary camera). Displacement of the spot center (orange) in the X (dashed) and λ (continuous) directions. Optimal DMD filters (middle panel) for supervised identification of polystyrene (PS), polymethylmethacrylate (PMMA) and water spectra (bottom panel).

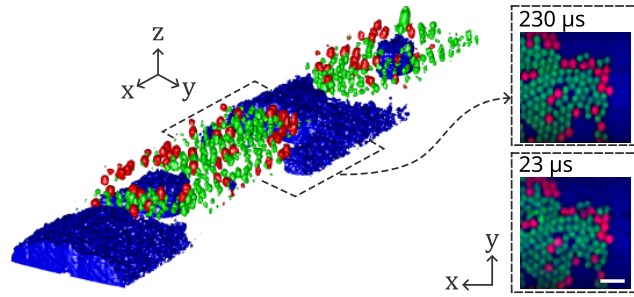


Figure 3. Compressive Raman image of beads made of PS (6 μm , red) and PMMA (5 μm , green) embedded in water (blue). The 3D rendering (left) is acquired at effective $\tau_{pdt} = 230 \mu\text{s}$. The two slices (right) correspond to 230 and 23 μs . Scale bar: 20 μm

to bottlenecks in data throughput (Kumamoto et al., 2022). *Effective* τ_{pdt} is defined as $\tau_{idt} \frac{N_{\text{DMD}}}{N_{\text{SPAD}}}$. The image acquired at effective $\tau_{pdt} = 23 \mu\text{s}$ ($\tau_{idt} = 1 \text{ ms}$, $N_{\text{SPAD}} = 128$) represents a 10 \times improvement in comparison with previous approaches (Scotté et al., 2019; Soldevila et al., 2019), despite significant losses in the layout (discussed below).

Further upgrades in the spectrometer and SPADs layout could increase this performance gain by at least 20 \times . We measured a $PDE_{\text{array}} = 7\%$, which can be increased to 20% with light-coupling microlenses, therefore improving the detection efficiency by 3 \times . Another 4-fold gain will be provided by using all 512 SPAD array pixels instead of the current $N_{\text{SPAD}} = 128$. An additional 2 \times factor can be achieved by using both DMD outputs (Rehrauer et al., 2018). We believe that further PSF engineering will enlarge the spectral bandwidth to cover also the fingerprint region, hence further improving spectral identification capabilities. Note that previous works have achieved $\tau_{pdt} = 5 \mu\text{s}$ for one filter (Rehrauer et al., 2018), however reaching the fundamental limit of the system, whereas the parallelized scheme presented here achieves for one filter 8 μs with much space for improvement.

In conclusion, we demonstrate that an effective parallelization of the single-pixel-based compressive Raman microscope allows to considerably increase the image acquisition. These results pave the way to video-rate imaging with the inexpensive spontaneous Raman effect. Perspectives

include label-free real-time biological or chemical identification solutions for applications such as histopathology and quality control.

References

- Bruschini, Claudio et al. (2019). "Single-photon avalanche diode imagers in biophotonics: review and outlook". In: *Light: Science & Applications* 8.1, p. 87. DOI: [10.1038/s41377-019-0191-5](https://doi.org/10.1038/s41377-019-0191-5).
- Burri, Samuel, Claudio Bruschini, and Edoardo Charbon (2017). "LinoSPAD: A Compact Linear SPAD Camera System with 64 FPGA-Based TDC Modules for Versatile 50 ps Resolution Time-Resolved Imaging". In: *Instruments* 1.1, p. 6. DOI: [10.3390/instruments1010006](https://doi.org/10.3390/instruments1010006).
- Cebeci, Derya, Bharat Mankani, and Dor Ben-Amotz (2018). "Recent Trends in Compressive Raman Spectroscopy Using DMD-Based Binary Detection". In: *Journal of Imaging* 5.1, p. 1. DOI: [10.3390/jimaging5010001](https://doi.org/10.3390/jimaging5010001).
- Corden, Christopher J. et al. (2018). "Fast Raman spectral mapping of highly fluorescing samples by time-gated spectral multiplexed detection". In: *Optics Letters* 43.23, p. 5733. DOI: [10.1364/ol.43.005733](https://doi.org/10.1364/ol.43.005733).
- Kumamoto, Yasuaki et al. (2022). "Slit-scanning Raman microscopy: Instrumentation and applications for molecular imaging of cell and tissue". In: *Journal of Applied Physics* 132.17. Publisher: AIP Publishing LLC/AIP Publishing, p. 171101. DOI: [10.1063/5.0102079](https://doi.org/10.1063/5.0102079).
- Lin, Haonan and Hilton B. De Aguiar (2021). "Compressive Raman microspectroscopy". In: *Stimulated Raman Scattering Microscopy: Techniques and Applications*. Elsevier, pp. 371–382. DOI: [10.1016/B978-0-323-85158-9.00036-1](https://doi.org/10.1016/B978-0-323-85158-9.00036-1).
- Lubin, Gur et al. (2021). "Heralded Spectroscopy Reveals Exciton-Exciton Correlations in Single Colloidal Quantum Dots". In: *Nano Letters* 21 (16), pp. 6756–6763. DOI: [10.1021/ACS.NANOLETT.1C01291/ASSET/IMAGES/LARGE/NL1C01291_0005.JPEG](https://doi.org/10.1021/ACS.NANOLETT.1C01291/ASSET/IMAGES/LARGE/NL1C01291_0005.JPEG).
- Réfrégier, Philippe et al. (2018). "Precision of proportion estimation with binary compressed Raman spectrum". In: *Journal of the Optical Society of America A* 35.1, p. 125. DOI: [10.1364/josaa.35.000125](https://doi.org/10.1364/josaa.35.000125).
- Rehrauer, Owen G. et al. (2018). "Binary Complementary Filters for Compressive Raman Spectroscopy". In: *Applied Spectroscopy* 72.1, pp. 69–78. DOI: [10.1177/0003702817732324](https://doi.org/10.1177/0003702817732324).
- Scotté, Camille et al. (2019). "Compressive Raman imaging with spatial frequency modulated illumination". In: *Opt. Lett.* 44.8, p. 1936. DOI: [10.1364/ol.44.001936](https://doi.org/10.1364/ol.44.001936).
- Scotté, Camille et al. (2020). "Line-scan Compressive Raman imaging with spatio-spectral encoding". In: *Opt. Lett.* 45.19, p. 5567. DOI: [10.1364/ol.400151](https://doi.org/10.1364/ol.400151).
- Soldevila, Fernando et al. (2019). "Fast compressive Raman bio-imaging via matrix completion". In: *Optica* 6.3, p. 341. DOI: [10.1364/optica.6.000341](https://doi.org/10.1364/optica.6.000341).
- Sturm, Benneth et al. (2019). "High-Sensitivity High-Speed Compressive Spectrometer for Raman Imaging". In: *ACS Photonics* 6.6, pp. 1409–1415. DOI: [10.1021/acsp Photonics.8b01643](https://doi.org/10.1021/acsp Photonics.8b01643).
- Wilcox, David S et al. (2012). "Photon level chemical classification using digital compressive detection". In: *Analytica Chimica Acta* 755, pp. 17–27. DOI: [10.1016/j.aca.2012.10.005](https://doi.org/10.1016/j.aca.2012.10.005).
- Wilcox, David S et al. (2013). "Digital compressive chemical quantitation and hyperspectral imaging". In: *Analyst* 138.17, pp. 4982–4990. DOI: [10.1039/c3an00309d](https://doi.org/10.1039/c3an00309d).