# Air-blood interface engineered microfluidic device to mimic shear rate gradient induced human bleeding model

Shobhit Das<sup>\*</sup>, Shilpi Pandey<sup>*α*</sup>, Oliver Hayden<sup>*α*</sup>

\* Indian Institute of Engineering Science and Technology, Shibpur, India <sup>α</sup> Technical University of Munich, Germany

# Abstract

Microfluidic technology has emerged as a powerful tool for studying complex biological processes with enhanced precision and control. This research paper presents a novel approach to replicate the bleeding model within a microfluidic chip to investigate the intricate dynamics of blood clots and platelet behaviour around the wound site. Leveraging the advantages of microfluidics, we aimed to bridge the gap between traditional animal models and human hemostasis, gaining insights into platelet-mediated clot formation during the critical stages of coagulation.

The microfluidic chip was designed to emulate human-like microvascular networks with precise control over channel geometry and flow conditions. By simulating blood flow dynamics during bleeding events, we successfully observed the real-time interactions of platelets and their aggregation induced by shear rate gradient at the wound site. Platelet dynamics is primarily influenced by physico-mechanical condition of blood vessels with pathophysiological condition of blood at close proximity of vascular injury site. This microfluidic platform facilitated the investigation of platelet adhesion, activation, and clot formation, providing a unique opportunity to study the spatiotemporal dynamics of platelet aggregation and blood clot.

Our findings shed light on the intricate mechanisms underlying thrombus formation and plateletmediated aggregation, offering a more accurate and dynamic representation of human haemostasis compared to traditional animal models. In the conventional approach, the human bleeding model is tried on mouse due to anatomy and pathological similarities between mouse and humans. This study will simplify and standardize the blood and vasculature conditions. The microfluidic-based replication of the bleeding model holds significant promise in advancing our understanding of clotting disorders and wound healing processes. Furthermore, it paves the way for targeted therapeutic interventions in managing bleeding disorders and enhancing clinical strategies for promoting efficient wound closure. Ultimately, this study demonstrates the potential of microfluidics to revolutionize haemostasis research and opens up new avenues for the development of personalized medicine approaches in the field of clotting disorders.

#### **Keywords**

Blood air interface - Blood analysis - Haemostasis - In vivo - Shear rate

#### 1. Introduction

Animal models have long been instrumental in studying haemostasis and blood clotting; however, complexity of vascular physiology have prompted researchers to explore alternative approaches [1]. Microfluidic technology has emerged as a powerful tool [2], offering a novel platform to mimic the intricate dynamics of blood flow and coagulation processes within a controlled environment.

The bleeding model has been a cornerstone in studying haemostasis due to the genetic similarities and physiological relevance between mice and humans [3][4]. However, extrapolating the findings to human haemostasis presents challenges, as differences in vascular anatomy, blood flow dynamics, and platelet function exist between species. Blood clotting at vascular injury site is subjective to vessel shear rate activated platelet aggregation and thrombus formation. By adopting a microfluidic-based approach, we can overcome these limitations and create a tailored bleeding model that accurately mimics human-like microvascular networks. Through precise control over channel geometry and flow conditions, we can simulate the dynamics of blood flow during bleeding events, offering a platform to observe the behaviour of platelets at the wound site. This microfluidic model provides a unique opportunity to observe the real-time interactions of platelets and their aggregation, offering insights into the underlying mechanisms governing clot formation.

Platelets, small anucleate cells, play a pivotal role in the primary phase of haemostasis by forming aggregates at the site of vascular injury, initiating the coagulation process [5]. Their interactions with the exposed extracellular matrix and other blood components contribute to the formation of a stable haemostatic plug. Microfluidic devices have been tailored to incorporate biochemical cues that mimic the physiological environment around the wound, promoting platelet adhesion and aggregation. Additionally, real-time imaging and advanced microscopy techniques within the microfluidic chip allow for detailed observation of platelet behaviour, enabling the quantification of critical parameters such as clotting time, clot size, and platelet activation levels. This comprehensive analysis of platelet blood coagulation within the microfluidic chip presents an unprecedented opportunity to unravel the intricacies of thrombus formation and explore potential therapeutic targets for clotting disorders.

In this research paper, we present a pioneering study that aims to replicate a bleeding model on a microfluidic chip to investigate the complex behaviour of platelets during blood coagulation around the wound. By leveraging the precision and versatility of microfluidics, we seek to shed light on the critical cellular and molecular events that govern haemostasis, opening up new avenues for understanding and potentially treating clotting disorders. From the experiment and COMSOL model it is clearly evident that the rather than hemostatic plug formation is "characterize" by extremely high shear, probably boosting platelets. In this process surface tension and uncontrolled vortex of suspended particles in blood also come into action. The study of platelets and coagulation will lead us to study the prevention of haemostatic and thrombotic diseases like haemophilia, Von Willebrand disease, Pulmonary embolism, stroke etc [6].

In the recent past, there have been certain breakthroughs in this field of research consisting thrombosis model and shear rate activated platelet aggregation. Several recent research papers have contributed valuable insights into shear rate-affected platelet aggregation, shedding light on the intricate relationship between blood flow dynamics and platelet function. Article by Lauren D. C. Casa et al. [7], they have discussed the effects of Von Willebrand factor and how it gets affected by changes in shear rate. A research paper by Warwick S Nesbitt et al. [5], has discussed how platelet aggregation is affected by changes in shear rate but In non-bleeding models in vivo and in vitro In 2018, a paper by Yumiko Sakurai [8] made a bleeding model by creating a thin PDMS flap valve between blood and air. They have cultured endothelial cells in the inner wall of the PDMS device but they have no text on direct air blood interface. In a review article, Trevisan et al. [6] have discussed various microfluidic techniques

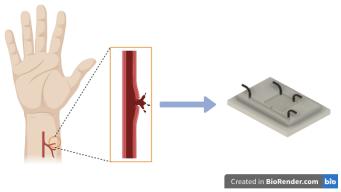


Figure 1: Illustration of the basic idea of our project

to study platelet activation and blood coagulation. Finally, agreeing in rectangular crossectional channels to study platelet activation and blood coagulation under adequate flow parameters. Despite this thorough advancement in the field of this research study, no documentation is available on the direct interaction of blood and air, which occurs during an injury. However, our in-vitro setting could potentially be used to test both situations i.e., external bleeding and internal bleeding.

In this research paper, we present the design and development of a microfluidic chip that replicates the bleeding model to investigate blood clot around the wound at the blood-air interface Fig.1. Through a series of experiments and imaging analyses, we aim to characterize the spatiotemporal dynamics of platelet aggregation, shedding light on the contributions of individual platelets to the haemostatic process. The insights gained from this microfluidic approach hold significant promise in advancing our knowledge of haemostasis and may pave the way for the development of targeted therapies to manage bleeding disorders and enhance wound healing in clinical settings. Creating an air pressure valve to control the wound opening is an important as well as innovative factor in our study.

## 2. Material and Methodology

#### 2.1 Microfluidic Chip Fabrication

This section describes the methodology and experimental procedures used for the fabrication of the microfluidic chip. Initially, a reverse replication of microfluidic chip design was realized on a silicon wafer using maskless laser patterning of SU8 photoresist on a silicon wafer and used as a master mold for transferring the pattern on Polydimethylsiloxane (PDMS). In this process a 3-inch wafer (Microchemical Ulm, Germany) was taken for microstructure patterning. First, silicon wafer was cleaned in acetone and isopropyl alcohol for 5 mins at 35 °C each in an ultrasonic bath, which was followed by drying using nitrogen, and a dehydration bake was given at 120 °C for 5 mins. SU8 3050 photoresist (Microchemical Company) was poured on the wafer and then spin-coated (spincoater.com) at 500 rpm for 10 seconds and then at 1000 rpm for 30 sec to achieve uniform thickness of SU8 on entire wafer surface with a height of 100 µm. The wafer is pre-baked at 65°C for 10 mins and at 95°C for 30 mins. After prebaking the photoresist was exposed to ultraviolet light using a mask-less laser writer to obtain a 3x3 array of reverse pattern of microfluidic chip as shown in Fig.2(a) followed by post-baking at 95°C for 5 mins to complete polymerisation process. Further, the pattern was developed using MIF 326 developer for 10 mins, then rinsed with IPA and acetone and dried with a nitrogen gun. The height of the reverse replication pattern was 100 µm as measured. Further, for replication of microfluidic chip on PDMS material, sylgard base and curing agent were mixed in a ratio of 10:1 and poured on the 3x3 array of patterns engraved on SU8 mastermold which was further degassed using vacuum pump for 40 min followed by curing in an oven at 65°C for 1 hour. The PDMS chip was then

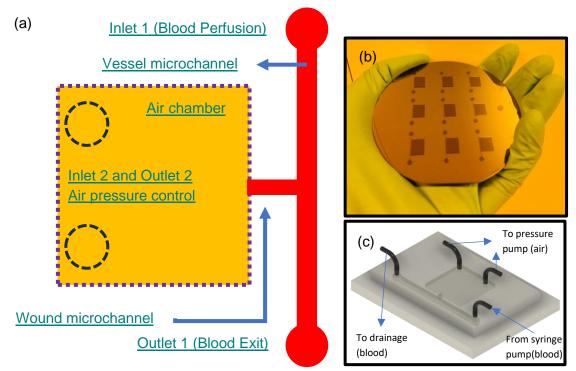


Figure 2: (a) The basic plan of our device including the wound Caliber, blood vessel and air chamber. (b) Design array on silicon wafer working as negative mould. (c) An illustration of the device with all connection made in Fusion 360

cut using a blade and gently peeled off from the SU-8 master. The inlet and the outlet of both blood channel and air chamber were punched using a 0.5 mm biopsy punch. Next, the chip was bonded to a glass slide using plasma bonding in plasma bonder (Diener Zepto Modell 8 Grundgerat Typ B) at an oxygen flow of 0.6 bar and at 50% power.

#### 2.2 Preparing blood sample

A trained phlebotomist collected blood from a healthy donor using an EDTA tube and kept it on the roller for 10-15 minutes before using the blood for the experiment. The blood was then mixed with antibodies (1:100 ratio) Antibody was an anti-human CD41 [plts-specific molecular marker] labelled with FITC [dye name]. Before the experiment, blood has been recalcified to 2.4mM by adding Calcium Chloride. following the Equation 1. The blood was used within 2-3 hours after collection [9].

$$V_f \times C_f = V_i \times C_i \tag{1}$$

Where V, C, f, i, are volume, concentration, final and initial, respectively. The whole setup of the experiment is kept at a stable equilibrium under a fluorescent microscope (Leica Model TL LED). The Fit-C filter (with an excitation frequency of 480-490nm and emission frequency of 510-520nm) is used during fluorescent imaging. Images and videos were captured with low-intensity light to avoid unnecessary activation of fluorescent dye. To analyse the videos retrieved from the microscope and plot the platelet deposition with respect to time a python code is used.

#### 2.3 Experimental Design and Procedure

Devices with different wound sizes were bonded on the same glass slide to conduct the experiment. A syringe pump (Chemyx Fusion 4000) containing the blood is connected to the inlet of the blood vessel with PLA micro tubing. A pressure pump (Fluigent Flow EZ) is connected to the inlet of the pressure

chamber to maintain the air pressure as depicted in Fig.2(c). Following theory, initially, the air pressure is maintained at air chamber at a certain level, and blood is perfused by the syringe pump. The additional air pressure is compensated to maintain air-blood interface at the junction point of the wound channel and blood vessel. The air pressure is then suddenly dropped to zero to replicate sudden haemorrhage of the blood vessel. As a result, blood flows out of the wound microchannel into the air chamber. The particular device on which the experiment is done is observed under the fluorescent microscope.

The basic idea of the microfluidic device is to manipulate the air blood interface by changing the air pressure in the air chamber and mimicking the dynamic of the wound. Initially, the air pressure is kept sufficient that the meniscus stays near the channel and subsequently mimics an unruptured blood vessel. Then the air of the chamber is decreased and the meniscus of the fluid moves towards the air chamber and after a specific threshold value, the liquid flows into the air chamber through the newly formed microchannel analogous to bleeding and also flows straight in the microchannel. All the data regarding the equilibrium air pressure, flow rate, and type of device used in different sets of experiments are mentioned in table 1.

# 3. COMSOL Model

In this section, we describe the specific setup and configuration of the COMSOL simulation used for the study. The simulation aims to model and analyse the behavior of the microfluidic chip and provide insights into its performance. A COMSOL (5.6) 2-phase, phase field model is used to simulate the experiment in COMSOL Multiphysics software. Two- phase model is exclusively chosen as there are two mediums in contact with each other. An air-blood interface is formed, which is very important for our experiment.

The vessel diameter is taken to be  $100 \ \mu m$ , which is similar to the vessel diameter we are using in the microfluidic chip. The wound caliber is made with another cylinder attached to the vessel periphery and at the other end of the wound a chamber is added with the air at atmospheric pressure. To optimize the simulation time, the dimension of the pressure chamber is shortened as compared to the microfluidic device. The user-control adaptive meshing technique is used for the meshing of the simulation. To optimize the simulation time and get accurate results, the meshing is kept ultra-fine near the wound and gradually becomes coarser as we move away from the wound.

For fluid-1, blood is considered, and for fluid-2, air is considered in the air chamber. Laminar flow is assumed. As the blood is just a suspension of erythrocytes, leukocytes, thrombocytes, etc. we considered an inelastic non-Newtonian fluid. Power Law in an elastic model with a fluid consistency coefficient of 0.016 and flow behavior index of 0.66 is considered. The focal governing equation of power law to calculate shear rate is given below Equation 2.

$$\tau = K (\frac{\delta u}{\delta y})^n \tag{2}$$

Where  $\tau$ , K,  $\frac{\delta u}{\delta y}$ , n, shear stress, flow consistency index ( $Pas^n$ ), velocity gradient perpendicular to the plane of the shear (s<sup>-1</sup>), respectively. The inlet velocity of blood in the vessel is taken to be 0.3 m/sec and the counter pressure at the output of the vessel is taken as 1013 Pa. There is also an outlet at the wound which is maintained at atmospheric pressure. The slip condition at all the walls is considered a no-slip condition.

Blood and air are used in the simulation and all the parameters of these two liquids are kept the same as in the model. For the time-dependent simulation, the time frame is kept at 1 second, and simulation steps are maintained every 0.01 seconds. The relative tolerance is maintained at 0.001. Velocity profile,

pressure, volume fraction of liquid 1 (blood), and shear rate are observed after computation to a remote desktop which has a RAM of 24GB.

#### 4. Results and Discussion

# 4.1 Effect of shear stress, surface tension and vortex of suspended particles in blood vessel

Microfluidic devices were developed with two different dimensions of the wound (15 and 50  $\mu$ m) as mentioned in Table 1. The height of the microchannels and the air chamber i.e., 100  $\mu$ m were kept constant for all devices, as shown in Fig.2(a). The experiment was performed on both devices. Initially, the air chamber pressure was controlled at equilibrium air pressure as mentioned in Table 1, then the blood was injected into the device at flow rate of 1  $\mu$ L/min. When blood starts flowing through the vessel/microfluidic channel due to the no-slip condition of the wall, shear gradient starts developing radially. Thus, we often see platelets sticking to the inner wall of the blood vessel [1]. This same phenomenon of radial shear gradient is also observed in COMSOL simulation, as shown in Fig.3(a) and Fig.3(b). As a matter of fact, we observe the endothelial cells elongated and attached to the inner wall of blood vessel. Due to shear gradient, which is originated by laminar flow, the exposed endothelial cells get elongated along the flow [6]. Thus, thrombocytes get activated due to different shear gradients at several points inside the microchannel and then get aggregated at the injury region.

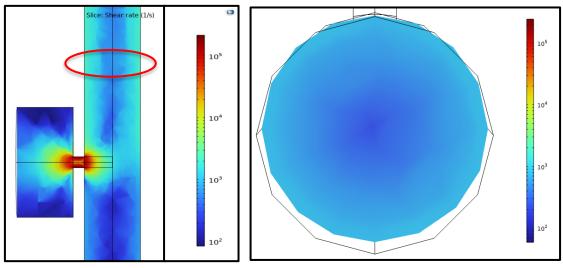


Figure 3: (a) The encircled region from the simulation result of logarithmic shear rate plot illustrates the radial change in shear rate. It is perceived that the radial change is due to the no-slip condition of the wall. (b) The radial distribution of the shear rate which shows similar characteristics to shear rate distribution in live blood vessel.

Table 1. This table highlights the parameters that are varies and their variation throughout the experiment
and the constant parameters

Device	Ideal	Actual	Ideal dimension	Actual	Equilibrium	Blood
No.	dimension of	dimension of	of vessel height	dimension of	air pressure	flow rate
	wound (µm)	wound (µm)	(µm)	vessel width	(mbar)	(ul/min)
				(µm)		
1	50	51.7±0.7	100	99.2±1.5	17.5±2.1	1
2	15	$14.52 \pm 1.1$	100	99.2±1.5	46±2.1.3	1

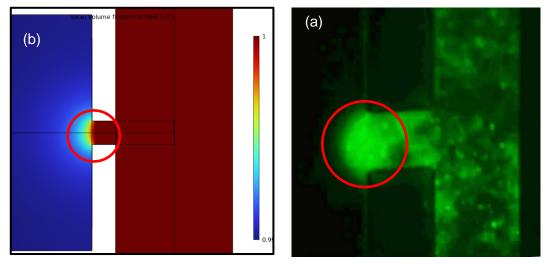


Figure 4: (a) Simulation result of volume fraction of blood at time = 0.14 sec also show an arcing at the same region of the wound. (b) Snapshot from experiment video having a arcing of the blood near the exit of the wound depicting that surface tension force is in action. The bright green area in the encircled region the aggregating of platelet due to the shear rate change from the effect of surface tension.

Further, as blood moves toward the opening of the wound in a microfluidic device, surface tension also plays an important role since dimensions are in the micro-meter range and viscous effect is dominating. Fig.4(a) and Fig.4(b) demonstrates the platelet distribution at wound site as observed through fluorescent microscopy and its comparison with simulation result. A bright green area as marked by circle clearly demonstrated the aggregation of platelet due to shear rate gradient. At the sight of a wound opening, initially, there is some resistance force on the blood flow, but as soon as the flow pressure reaches a certain threshold, the force of surface tension is overcome, and then the blood drifts out from the wound opening. The arcing profile of blood Fig.4(a) due to surface tension is also retrieved from the COMSOL simulation. The inertial force of the suspended particles makes them flow towards the air-blood interface: wound opening, but due to very limited inertial force, the particles tend to stay there, surrendering to the surface tension. Due to this, thrombocytes start accumulating at the sight of the wound opening, which is observed during the experiment, highlighted in fluorescent green Fig.4(b). Blood is a heterogeneous mixture of numerous types of cells and molecules that contain different momentum. Due to this dynamic range of cells available in the blood, when the vessel is ruptured, there

is a possibility of eddy generating at the entry of the wound, the same we observed in the experiment

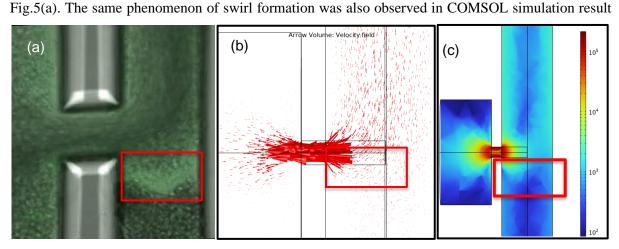


Figure 5: (a) Experimental result highlighting the effect of swirling motion near the injury calibre. (b) simulation result showing proportionate arrow volume for velocity plot also satisfying the effect of eddy. (c) Shear rate plot in logarithmic scale also showing a shear rate gradient near the eddy region.

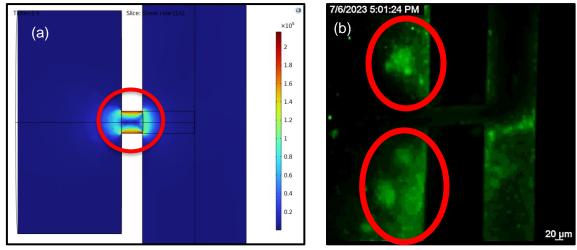


Figure 6: (a) Represent the simulation, and the red encircled region denote the area of maximum shear change. (b) Image captured during the experiment where the red encircled region with the green highlighting depicts the region of platelet aggregation.

Fig.5(b) when we plot the tangential velocity for each node. Due to this swirl, the change in shear rate, causes the platelet to activate and aggregate at that region of the vessel, as shown in Fig.5(c). However, it is different with real-world scenarios i.e., blood vessels present in our body. In our body when there is injury or sudden opening in the blood vessel due to foreign force, the vessel swells due to inflammation at that region, creating an adequate cross-sectional area for the blood to flow straight through the vessel. The swelling of the blood vessel reduces the swirl and its effect on the injury section. In the PDMS-based microfluidic device, as there is no swelling, the eddy of the suspended particles is visible clearly Fig.5(a).

Further, when blood flows out of the wound opening, we have observed, experimentally and in COMSOL simulation, a significant change in the shear rate near the wound region Fig.6(a), highlighted with red circle). The change in shear rate builds a shear gradient around that region, eventually activating the platelets. The green deposition encircled in red in Fig.6(b) confirms the area where the platelets are getting deposited. Under the normalized situation, the platelet aggregates encircling the wound opening and slowly and eventually covering the wound to stop the bleeding. We have observed the lumps of activated platelets all along the blood flow region, and due to the absence of collagen, the activated platelets get collectively settled in the next equilibrium wall after the high shear rate region. In the in-vivo model, during activation, the platelets grow finger-like projection that helps the platelets to bind with collagen and also among themselves as shown in Fig.7(a) and Fig.7(b). Since there was no collagen present on the inner wall of PDMS, no bond was possible between the platelets and the PDMS wall, which is contrary to the fact that in our body the platelets bond with the inner wall of blood vessels with the help of  $\alpha 2\beta 6$ , GPVI, and Von-Willebrand factors. Von Willebrand only gets activated at an excessive shear rate [7][8].

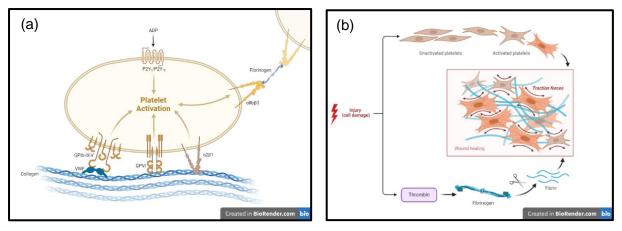


Figure 7: (a) An illustration highlighting the bonding characteristics of platelets with collagen with the help of different factors and the bonding between 2 platelets with the help of fibrinogen. (b) An illustration highlighting the whole process of platelet aggregation. During activation the platelet grows finger like projection which benefit them to bind among themselves with the help of fibrinogen molecule.

#### 4.2 Image analysis

As shown in Fig. 9, for device 1 with wound size 50  $\mu$ m, platelet deposition is gradually increasing with respect to time once the blood start flowing through the would caliber, which is the natural tendency of the platelet deposition i.e., the extent of platelet deposition increases as time passes. For another device, it is perceived that as the wound dimension is 15  $\mu$ m, the velocity of blood coming out of the wound is sufficiently high. As the flow rate of 1  $\mu$ l/min is kept constant for both devices, cross-sectional area and velocity are inversely proportional; thus, for a device with 15  $\mu$ m wound size, we achieve the high velocity of blood flowing out of the wound. This velocity is sufficiently high enough to carry the aggregated platelets away from the wound site. Due to this understanding, the graph shows a constant behaviour rather than increasing or decreasing tendency.

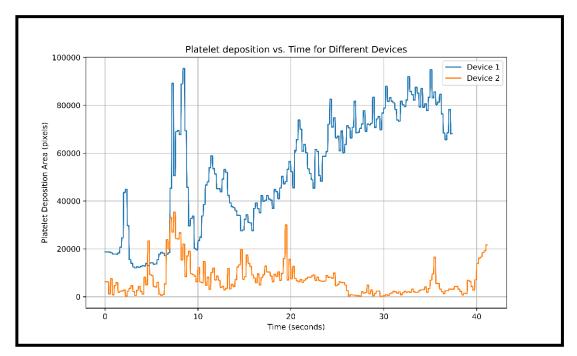


Figure 8: Data retrieved from the experimental videos visualising the amount the platelet aggregation with respect to time for Device 1 and 2.

# 5. Conclusion

As per our observation, it is evident that the shear rate near the wound region is extremely high as compared to other parts of the microfluidic channel. Due to this sudden change in shear rate, the platelets get activated and bind together at the injury site and enhancing platelet binding to the inner wall. An understanding is also developed of the mild shear rate change due to the swirling of suspended particles in the blood. An additional inference made from the simulation and [10] is that due to radial shear gradient platelets aggregate near the wall and additionally attract other platelets near them as well. Another inference from our investigation is that at the larger dimension of the wound (i.e., for the lower outward velocity of blood) the platelets tend to stick to the wall but for the lesser dimension of the wound (when the outward velocity is high) the lumps of platelets tend to flow away with the blood flow thus reducing aggregation efficiency.

Additional to this we have also come to a conclusion that if we swap air with other liquid which validates similar properties of different biofluids, we can also simulate internal bleeding where the blood vessel ruptures and the blood comes in contact with several biofluids directly. Thus, with our device we can study external as well as internal bleeding.

# 6. Acknowledgement

Shobhit Das would like to extend his sincere gratitude to the German Academic Exchange Service (DAAD) for their generous support through the WISE program, which made his internship trip to the Technical University of Munich (TUM), Germany, possible. We are also deeply appreciative of TranslaTUM and Ludwig Maximilian University of Munich (LMU) for providing access to their exceptional lab facilities, which significantly contributed to the quality and depth of my research work. I extend my heartfelt thanks to Prof. Dr. Ghulam Gestgeer for his invaluable assistance in developing the COMSOL model, and to Freidrich Deemann for his expert guidance and support during the experimental phase of my research. We want to express our gratitude

## 7. References

- [1] Stalker, T.J., 2020. Mouse models of platelet function in vivo. Platelets, 31(4), pp.415-416
- [2] Pandey, S., Mehendale, N. and Paul, D., 2021. Single-Cell Separation. In *Handbook of Single-Cell Technologies* (pp. 207-234). Singapore: Springer Singapore
- [3] Panteleev, M.A., Korin, N., Reesink, K.D., Bark, D.L., Cosemans, J.M., Gardiner, E.E. and Mangin, P.H., 2021. Wall shear rates in human and mouse arteries: Standardization of hemodynamics for in vitro blood flow assays: Communication from the ISTH SSC subcommittee on biorheology. *Journal of Thrombosis and Haemostasis*, 19(2), pp.588-595.
- [4] Mohammed, B.M., Monroe, D.M. and Gailani, D., 2020. Mouse models of hemostasis. *Platelets*, 31(4), pp.417-422.
- [5] Nesbitt, W.S., Westein, E., Tovar-Lopez, F.J., Tolouei, E., Mitchell, A., Fu, J., Carberry, J., Fouras, A. and Jackson, S.P., 2009. A shear gradient–dependent platelet aggregation mechanism drives thrombus formation. *Nature medicine*, 15(6), pp.665-673.
- [6] Trevisan, B.M., Porada, C.D., Atala, A. and Almeida-Porada, G., 2021, April. Microfluidic devices for studying coagulation biology. In *Seminars in cell & developmental biology* (Vol. 112, pp. 1-7). Academic Press.

- [7] Casa, L.D., Deaton, D.H. and Ku, D.N., 2015. Role of high shear rate in thrombosis. *Journal of vascular surgery*, *61*(4), pp.1068-1080.
- [8] Sakurai, Y., Hardy, E.T., Ahn, B., Tran, R., Fay, M.E., Ciciliano, J.C., Mannino, R.G., Myers, D.R., Qiu, Y., Carden, M.A. and Baldwin, W.H., 2018. A microengineered vascularized bleeding model that integrates the principal components of hemostasis. *Nature communications*, 9(1), p.509.
- [9] Cabrera, D., Walker, K., Moise, S., Telling, N.D. and Harper, A.G., 2020. Controlling human platelet activation with calcium-binding nanoparticles. *Nano research*, *13*, pp.2697-2705.
- [10] Zelená, A., Isbaner, S., Ruhlandt, D., Chizhik, A., Cassini, C., Klymchenko, A.S., Enderlein, J., Chizhik, A. and Köster, S., 2020. Time-resolved MIET measurements of blood platelet spreading and adhesion. *Nanoscale*, 12(41), pp.21306-21315.