

1 **Measuring joint kinematics of treadmill walking and running:**
2 **comparison between an inertial sensor based system and a camera-based system**

3
4 Corina Nüesch^{1,2}
5 Elena Roos^{1,3}
6 Geert Pagenstert¹
7 Annegret Mündermann^{1,2}

8
9 ¹Clinic for Orthopaedics and Traumatology, University Hospital Basel, Basel, Switzerland

10 ²Department of Biomedical Engineering, University of Basel, Basel, Switzerland

11 ³Department of Health Sciences and Technology, ETH Zurich, Zurich, Switzerland

12
13
14 *Original Article*

15
16
17 Nüesch C., E. Roos, G. Pagenstert, and A. Mündermann (2017) Measuring joint kinematics of
18 treadmill walking and running: comparison between an inertial sensor based system and a
19 camera-based system. Journal of Biomechanics 57:32-38. DOI:
20 [10.1016/j.jbiomech.2017.03.015](https://doi.org/10.1016/j.jbiomech.2017.03.015). This work is licensed under a [Creative Commons](https://creativecommons.org/licenses/by/4.0/)
21 [Attribution 4.0 International License](https://creativecommons.org/licenses/by/4.0/).

22
23
24
25 Address for Correspondence: Dr. Corina Nüesch
26 Clinic for Orthopaedics and Traumatology
27 University Hospital Basel
28 Spitalstrasse 21
29 4031 Basel, Switzerland
30 Tel. +41 61 265 9444
31 Email corina.nueesch@usb.ch

32
33
34 Key words: inertial sensors; kinematics; walking; running; agreement

35
36
37 Word count: 3419 (Abstract: 250)

39 **Abstract**

40 Inertial sensor systems are becoming increasingly popular for gait analysis because
41 their use is simple and time efficient. This study aimed to compare joint kinematics measured
42 by the inertial sensor system RehaGait[®] with those of an optoelectronic system (Vicon[®]) for
43 treadmill walking and running. Additionally, the test re-test repeatability of kinematic
44 waveforms and discrete parameters for the RehaGait[®] was investigated. Twenty healthy
45 runners participated in this study. Inertial sensors and reflective markers (PlugIn Gait) were
46 attached according to respective guidelines. The two systems were started manually at the
47 same time. Twenty consecutive strides for walking and running were recorded and each
48 software calculated sagittal plane ankle, knee and hip kinematics. Measurements were
49 repeated after 20 minutes. Ensemble means were analyzed calculating coefficients of multiple
50 correlation for waveforms and root mean square errors (RMSE) for waveforms and discrete
51 parameters. After correcting the offset between waveforms, the two systems/models showed
52 good agreement with coefficients of multiple correlation above 0.950 for walking and
53 running. RMSE of the waveforms were below 5° for walking and below 8° for running.
54 RMSE for ranges of motion were between 4° and 9° for walking and running. Repeatability
55 analysis of waveforms showed very good to excellent coefficients of multiple correlation
56 (>0.937) and RMSE of 3° for walking and 3° to 7° for running. These results indicate that in
57 healthy subjects sagittal plane joint kinematics measured with the RehaGait[®] are comparable
58 to those using a Vicon[®] system/model and that the measured kinematics have a good
59 repeatability, especially for walking.

60

61

62 **Introduction**

63 Gait analysis is an important tool for objectively assessing gait function by providing
64 information on spatiotemporal parameters (e.g. step length, step time, length of stance phase)
65 and lower extremity joint kinematics, kinetics and muscle activation. However, conventional
66 instrumented three-dimensional gait analyses with simultaneous measurements with cameras,
67 force plates and electromyography is costly and time consuming. Technological advances
68 have facilitated development of alternatives to such laboratory based analyses. In recent years,
69 the popularity of inertial sensor based motion analysis systems for assessing joint kinematics
70 has increased (Hamacher et al., 2014; Sprager and Juric, 2015) with the advantage of simple
71 and time efficient gait analyses outside of the laboratory environment.

72 For instance, the RehaGait[®] system/model includes seven inertial sensors and software
73 that calculates spatiotemporal parameters and sagittal ankle, knee and hip kinematics. This
74 system has good reliability for spatiotemporal variables and the minimal foot-to-ground angle
75 with intraclass correlation coefficients (ICC) between 0.874 and 0.948 (Schwesig et al.,
76 2010). Spatiotemporal variables measured using an inertial sensor system showed good
77 agreement with those measured using an instrumented treadmill with average ICCs above
78 0.897 (Donath et al., 2016). Similar data on comparison of kinematic data of the RehaGait[®]
79 system/model and of an optoelectronic system/model during walking and running are
80 currently lacking.

81 The concurrent validity of kinematic data presumably depends on the specific
82 combination of inertial sensors and models. Initial results for other inertial sensor based
83 systems/models were promising where kinematic data measured from an inertial sensor
84 system and kinematic data measured through marker clusters at the same position as the
85 inertial sensor were interchangeable (e.g. “Outwalk” or “Cast” with Xsens[®] or Vicon[®];
86 coefficient of multiple correlation for sagittal ankle, knee and hip kinematics >0.95) (Ferrari
87 et al., 2010b). The results were even better when the offset between the systems/models was

88 corrected. Moreover, high correlations between calculated joint angles of another system
89 compared to the ones of a marker based model were reported (>0.80) for the sagittal knee and
90 hip angle, but correlations were low (<0.10) for the sagittal ankle angle during walking at
91 normal speed (Cloete and Scheffer, 2008). The reported average root mean squared errors
92 (RMSE) in the sagittal plane ranged from 10° to 20° for the calculated data and from 5° to 12°
93 after correcting the offset (Cloete and Scheffer, 2008). In contrast, another study (Picerno et
94 al., 2008) reported small differences (RMSE $<5^\circ$) for three-dimensional ankle, knee and hip
95 kinematics during walking between inertial and magnetic sensors combined with an
96 anatomical landmark calibration and a marker based model.

97 The primary aim of this study was to compare the joint kinematics measured by the
98 inertial sensor system RehaGait[®] with those of a commonly used clinical optoelectronic
99 protocol for treadmill walking and running. We hypothesized that the sagittal plane
100 kinematics of the two systems/models would be highly correlated and that there would be no
101 differences between discrete parameters (minimum/maximum values, range of motion)
102 calculated from the kinematic waveforms of the two systems/models. The secondary aim of
103 the study was to investigate the test-retest repeatability of the kinematic waveforms and the
104 discrete parameters measured by the inertial sensor system/model.

105

106 **Methods**

107 *Participants*

108 Twenty healthy subjects (12 female; age: 27.4 ± 8.3 years; height: 1.75 ± 0.08 m; body
109 mass: 66.5 ± 12.5 kg; body mass index: 21.5 ± 2.5 kg/m²) participated in this study. Exclusion
110 criteria were pain and/or lower leg injuries within the last 6 months. All subjects were
111 experienced runners with a weekly mileage of 45 ± 20 km/week. The study was approved by
112 the local ethical committee and all subjects signed informed consent forms prior to
113 participation.

114

115 *Procedures and data processing*

116 All subjects performed a walking and running analysis at their self-selected comfortable
117 speed on an instrumented treadmill (hp/cosmos mercury; Zebris, Isny, Germany) wearing
118 their preferred running shoe. Kinematic data were collected using two independent systems
119 and models – inertial sensor based and optoelectronic based – that were manually started at
120 the same time.

121

122 *Inertial sensor system and model.* The inertial sensor system (RehaGait[®], Hasomed,
123 Magdeburg, Germany) consists of seven inertial sensors each comprising a triaxial
124 accelerometer (± 16 g), a triaxial gyroscope (± 2000 °/s) and a triaxial magnetometer (± 1.3
125 Gs). The sensors were placed on the sacrum and bilaterally on the lateral thigh (middle),
126 lateral shank (lower third), and lateral foot (on the shoe, below lateral malleolus) using double
127 sided tape and elastic straps (Figure 1). The manufacturer's software and model was used to
128 calculate ankle, knee and hip angles in the sagittal plane with a sampling frequency of 400
129 Hz. The system and model are calibrated while the subject is in a neutral upright standing
130 position for 10 s and performs a slight squatting movement according to the manufacturer's
131 instructions. Hip extension is defined as positive and hip flexion as negative angles, and hence
132 all hip angles were multiplied by -1 to be consistent with the calculated angles from the
133 optoelectronic reference system.

134

135 *Optoelectronic system and model.* The optoelectronic system consisted of a 6-camera
136 motion analysis system (Vicon MX, Vicon Motion Systems Ltd., Oxford, UK) and 16
137 reflective markers that were placed on anatomical landmarks according to the PlugIn Gait
138 model – bilaterally on the posterior superior iliac spine, anterior superior iliac spine, lateral
139 thigh, lateral epicondyle of the knee, lateral shank, lateral malleolus, heel and second

140 metatarsal head (Kadaba et al., 1990). The infrared cameras tracked three-dimensional marker
141 positions with a sampling frequency of 200 Hz. The Nexus software and PlugIn Gait model
142 (Version 1.8.5, Vicon Motion Systems Ltd., Oxford, UK) were used to calculate three-
143 dimensional kinematics of the ankle, knee and hip joint. A static calibration trial in neutral
144 upright standing position was recorded before the dynamic walking and running trials.

145

146 After all sensors and markers were attached to the lower extremity, subjects first walked
147 on the treadmill for 30 s at their self-selected comfortable walking speed (for walking 1 hour).
148 Subsequently, data collection was initiated and kinematic data were recorded simultaneously
149 with both systems for 20 consecutive walking strides. The treadmill speed was then increased
150 to the self-selected running speed (comfortable running speed for 45 minutes) and subjects ran
151 for 3 minutes to adopt their regular running style before kinematic data were recorded with
152 both systems for 20 consecutive running strides (right foot strike to right foot strike).

153 To test the repeatability of the inertial sensor system/model, the entire setup including
154 inertial sensor placement and measurement procedure was repeated for walking and running
155 after 20 minutes.

156

157 *Data analysis*

158 The recorded waveforms for all sagittal plane kinematics of the ankle, knee and hip
159 joint for both measurement system/models were cut into strides by defining the minimum
160 knee angle after the swing phase as initial contact for both walking and running (Fellin et al.,
161 2010). All strides were time normalized to 0 to 100% beginning and ending at initial contact.
162 For each subject, system and joint, the ensemble means of angle waveforms and of peak joint
163 angles of 20 strides were calculated and used for further analysis. Discrete parameters were
164 calculated for the 20 strides of the two measurement systems/models as follows (Figure 2):
165 ankle angle at initial contact, first minimal ankle angle, maximal ankle angle, second minimal

166 ankle angle, difference between the maximal and the first minimal ankle angle (dorsiflexion
167 range of motion), difference between the maximal and the second minimal ankle angle
168 (plantarflexion range of motion), knee joint angle at initial contact, first maximal knee joint
169 angle, second maximal knee joint angle, minimal knee angle between the first and second
170 maximum, difference between the first maximal and the minimal knee angle (range of motion
171 first half stride), difference between the second maximal and the minimal knee angle (range of
172 motion second half stride), hip angle at initial contact, minimal hip angle, first maximal hip
173 angle, second maximal hip angle, difference between first maximal and minimal hip angle
174 (range of motion first half stride), and difference between minimal and second maximal hip
175 angle (range of motion second half stride).

176

177 *Statistical analysis*

178 All statistical analyses were performed in SPSS version 22.0 (IBM Corporation,
179 Armonk, NY) and Matlab (Version 2010a, MathWorks Inc., Natick, MA). To compare the
180 joint kinematics calculated from the RehaGait[®] system with the reference system the
181 following parameters were calculated: RMSE and coefficient of multiple correlation (Ferrari
182 et al., 2010a). RMSE of the waveforms was calculated with the ensemble mean data for each
183 subject and then averaged across joint and condition. The following interpretation of
184 coefficient of multiple correlation was used (Ferrari et al., 2010b): weak (<0.65); moderate
185 (0.65–0.75); good (0.75–0.85); very good (0.85–0.95); excellent (>0.95). This analysis was
186 repeated after removing the offset between the kinematic waveforms of the two
187 systems/models by centering each waveform on its respective mean (i.e. subtracting the mean
188 of a waveform from the entire waveform). The same parameters were calculated for the test
189 re-test repeatability of the RehaGait[®] system/model. Additionally, ICC with a two-way
190 random model for consistency and the systematic bias (mean difference between
191 measurements) with 95% limits of agreement ($1.96 * \text{standard deviation of the difference}$

192 between measurements) depicted as Bland and Altman plots were calculated for the ranges of
193 motion in walking and running. ICC were rated as excellent (0.9–1), good (0.74–0.89),
194 moderate (0.4–0.73), and poor (0–0.39) (Fleiss, 1986).

195 To reduce the complexity of the statistical analyses, only data of the right limb were
196 analyzed. Statistically significant differences in discrete kinematic parameters between
197 systems and models were detected using general linear models with factors time and system
198 and with Bonferroni correction to account for multiple parameters (significance level alpha:
199 $0.050/18 = 0.003$) with least square distance post hoc tests.

200

201 **Results**

202 *Walking*

203 The mean self-selected walking speed was 1.37 ± 0.13 m/s. There was a good
204 agreement between the average kinematic waveforms measured with the RehaGait[®] and the
205 reference system/model with very good to excellent coefficients of multiple correlation
206 (Figure 2). Removing the offset between the kinematic waveforms of the two systems/models
207 resulted in excellent coefficients of multiple correlation for all joints (between 0.967 and
208 0.988). The average RMSE between the original waveforms measured by the two
209 systems/models was smaller than 5° for the ankle joint and between 7° and 9° for the knee
210 and hip joint. After offset correction, the RMSE was smaller than 5° for all joints (Table 1).

211 The RMSE of the discrete parameters between the RehaGait[®] and the reference
212 system/model ranged from 4° to 9° for the ranges of motion and from 4° to 15° for the other
213 parameters (Table 2). For the ankle joint the RehaGait[®] system/model measured significantly
214 greater plantarflexion after initial contact and a significantly greater range of motion in the
215 stance phase than the reference system/model, while the other parameters showed no
216 statistically significant differences. Knee flexion angle at initial contact and peak knee flexion
217 angle during stance were significantly smaller and range of motion during swing significantly

218 greater with the RehaGait[®] than with the reference system/model. For the hip joint, all
219 discrete parameters were significantly different between the two systems/models (Figure 3,
220 Table 3).

221

222 *Running*

223 The self-selected running speed was on average 2.93 ± 0.35 m/s. For running, the
224 coefficient of multiple correlation between the knee kinematics measured with the RehaGait[®]
225 system/model and the reference system/model was very good, while the coefficient of
226 multiple correlation was moderate for the ankle kinematics and weak for the hip kinematics
227 (Figure 2). However, Figure 2 clearly shows an offset between the waveforms of the two
228 systems/models and removing this offset resulted in excellent coefficients of multiple
229 correlation for all joints (between 0.956 and 0.977). For all joints, the RMSE was between 18°
230 and 28° for the waveforms without offset correction and between 5° and 8° for the waveforms
231 with offset correction (Table 1).

232 The RMSE of the calculated ranges of motion in the three joints ranged from 4° to 9°,
233 while the RMSE of the other discrete parameters ranged from 13° to 36° (Table 2). The range
234 of motion of the ankle during stance and swing and of the knee and hip during swing did not
235 differ between the systems/models, while the knee and hip range of motion during stance
236 were significantly smaller when measured with the RehaGait[®]. The offset between the
237 waveforms showed that measurements with the RehaGait[®] system/model resulted in more
238 ankle plantarflexion, knee extension, and hip extension compared to the reference
239 system/model (Figure 3, Table 4).

240

241 *Repeatability RehaGait[®]*

242 The coefficient of multiple correlation of the kinematic waveforms was excellent for all
243 joints for walking (between 0.959 and 0.994). For running, the coefficient of multiple

244 correlation was very good for the ankle (0.937) and excellent for the knee and hip joint
245 (>0.984). The RMSE of the waveforms measured by the two systems/models was around 3°
246 for walking and between 3° and 7° for running (Table 1).

247 For walking, the RMSE of the discrete parameters between the RehaGait®
248 measurements ranged from 0° to 5°. For running, the RMSE ranged from 1° to 10° with the
249 highest RMSE occurring for the ankle range of motion during swing phase (Table 2). Except
250 for the minimal knee angle around foot off during walking, there were no significant
251 differences between the discrete parameters measured during the two measurements with the
252 RehaGait® for both walking and running (Table 3, Table 4). Limits of agreement were larger
253 for running than walking (Figure 3). For the ranges of motion, ICCs were good or excellent
254 for ankle, knee in the second half of the stride, and hip during walking and good or excellent
255 for ankle dorsiflexion, knee in the second half of the stride and hip during running (Figure 3).

256

257 **Discussion**

258 The primary aim of this study was to assess the agreement between sagittal plane joint
259 kinematics measured by the inertial sensor system RehaGait® and an optoelectronic system
260 during walking and running. Our results showed that the joint angles measured by the two
261 systems/models were highly correlated, but only after offset correction. The hypothesis that
262 there were no significant differences between discrete kinematic parameters between the two
263 systems/models had to be rejected for most parameters. The secondary aim of the study was
264 to investigate the test-retest repeatability of the kinematic waveforms and the discrete
265 parameters measured by the inertial sensor system/model. The results of this analysis showed
266 very good to excellent correlations between the test and re-test measurements with the
267 RehaGait® system/model and – except for the minimal knee angle around foot off during
268 walking – no significant differences between the discrete parameters measured in the test and
269 re-test sessions.

270

271 *Waveforms*

272 The inertial sensor based system/model and optoelectronic system/model used different
273 models to calculate kinematics. Previous research for the knee joint angle showed high
274 correlations and small RMSE ($<3.4^\circ$) for walking and running when kinematics were
275 calculated from the segment position data of inertial sensors and marker clusters using the
276 same models (Cooper et al., 2009; Favre et al., 2008; Picerno et al., 2008). The RMSE of the
277 waveforms were smaller than in our study. However, in studies that used independent models
278 to calculate kinematics from inertial systems/models and optoelectronic systems/models very
279 good to excellent correlations but higher RMSEs of 6° to 11° with offset correction and of up
280 to 20° without offset correction were reported (Cloete and Scheffer, 2008; Ferrari et al.,
281 2010b; Takeda et al., 2009). These results are comparable to our results and further emphasize
282 the importance not only of the source of position or movement data (inertial sensor versus
283 cameras) but also of the models used for measuring and calculating joint angles.

284 Most previous studies reporting good correlations between sagittal plane waveforms
285 measured by an inertial sensor system/model and model and an optoelectronic system/model
286 and model used correlation coefficients to compare their similarity (Cloete and Scheffer,
287 2008; Jaysrichai et al., 2015; Takeda et al., 2009). We used the coefficient of multiple
288 correlation as described by Ferrari (Ferrari et al., 2010a) because it considers the offset
289 between the waveforms, hence, explaining the lower correlation in our study compared to
290 some previous studies. The offset between the waveforms was greater for running than for
291 walking, thus partly explaining the lower coefficients of multiple correlation for running. The
292 RehaGait[®] model uses boundary conditions (i.e. knee angle is set to 0° at each initial contact)
293 to deal with the sensor drift during measurements. It is possible, that these boundary
294 conditions are met at a different time point during the stride or at a different joint position for
295 running than for walking, thus increasing the offset between the waveforms.

296

297 *Discrete Parameters*

298 To characterize gait or running patterns, discrete parameters such as minimal and
299 maximal angles or ranges of motion are often calculated. Our results showed that the two
300 systems/models RehaGait[®] and Vicon[®] yield significantly different discrete parameters. As
301 described for the waveforms, there was an offset between the systems/models explaining
302 some of the differences in minimal and maximal joint angles. This indicates that the discrete
303 parameters cannot be directly compared between the RehaGait[®] inertial sensor system/model
304 and optoelectronic Vicon[®] system/model. Moreover, we also observed systematic differences
305 in the ranges of motion parameters. These could be related to differences in the positioning of
306 sensors and markers and thus in segment positions, and to different definitions of joint axes.
307 For instance, the inertial sensor model uses a technical coordinate system without anatomical
308 information and the PlugIn Gait model uses an anatomical coordinate system. Furthermore,
309 soft tissue movement especially during running might influence marker and sensor positions
310 differently (i.e. due to difference in size or location on the leg), hence increasing differences
311 between the systems/models. Differences in the peak values, but not ranges of motion
312 measured by the two systems/models were greater for running than walking. This is likely
313 related to differences in the offset between the systems.

314

315 *Repeatability RehaGait[®]*

316 The coefficients of multiple correlation between the test and re-test RehaGait[®]
317 measurements were very good to excellent which is comparable to the results of a systematic
318 review on the reliability of optoelectronic three-dimensional gait analysis (McGinley et al.,
319 2009). For walking the RMSE of the waveforms was around 3° between the test and re-test
320 measurements, which also lies within the 2° to 5° that are reported for optoelectronic gait
321 analyses (McGinley et al., 2009). There were significant differences between the test and re-

322 test measurements for many of the discrete parameters. However, for the ranges of motion
323 during walking the limits of agreement were comparable to those reported in the literature for
324 optoelectronic gait analysis (Meldrum et al., 2014). Hence, the repeatability of the RehaGait®
325 system/model for walking is comparable to repeatability of optoelectronic systems/models
326 and suggests a clinically acceptable repeatability. Because the RMSEs were larger for running
327 than walking (especially in the second half of the stride, thus the swing phase), more caution
328 is needed for the interpretation of running measurements, particularly for the swing phase that
329 occurs in the second half of the stride.

330

331 *Limitations*

332 For both systems/models, the time of initial contact was determined from the knee
333 flexion/extension angle. Differences in this angle between the systems/models might translate
334 to slight differences in the time point of the initial contact between systems/models and
335 consequently also a time shift in the waveforms. Such a time shift could affect the coefficients
336 of multiple correlation and the joint angles at initial contact, but not range of motion
337 parameters. The RehaGait® and the optoelectronic system/model measured with different
338 sampling rates which could further influence the results on the agreement between the
339 systems/models. Moreover, averaging decreases the influence of possibly not analyzing the
340 same 20 strides of the two systems, because systems were manually started at the same time
341 but not synchronized. The data was collected for walking and running on a treadmill in
342 healthy subjects. It remains to be determined if a comparison of the RehaGait® system/model
343 with an optoelectronic reference system/model during overground walking and running yields
344 similar results. However, treadmill gait analysis is frequently utilized in clinical practice and
345 by therapists and coaches, and hence the results of this study are highly relevant.

346

347 *Conclusion*

348 This study showed that for healthy subjects the sagittal plane joint kinematic waveforms
349 measured with the RehaGait[®] inertial sensor system/model are comparable to those of a
350 Vicon[®] optoelectronic reference system. Because of an offset between the systems/models,
351 discrete parameters cannot be compared directly. The application of this inertial sensor system
352 is easy and less time consuming than that of the optoelectronic system. The repeatability of
353 the RehaGait[®] system/model was better for walking than running. Our results showed that the
354 RehaGait[®] system/model provides important and relevant information on gait patterns with
355 clinically acceptable repeatability for treadmill walking and the stance phase, but not the
356 swing phase of running.

357

358 **Conflict of interest statement**

359 The authors declare no conflict of interest.

360

361 **Acknowledgement**

362 The authors thank Nils Altrogge for his assistance in data collection. This study was
363 funded in part by the Swiss National Science Foundation (SNSF #32003B_159871/1).

364

365 **References**

366 Cloete, T., Scheffer, C., 2008. Benchmarking of a full-body inertial motion capture system for
367 clinical gait analysis. In: *2008 30th Annual International Conference of the IEEE*

368 *Engineering in Medicine and Biology Society: 2008*: 4579-4582.

369 Cooper, G., Sheret, I., McMillian, L., Siliverdis, K., Sha, N., Hodgins, D., Kenney, L.,

370 Howard, D., 2009. Inertial sensor-based knee flexion/extension angle estimation. 42,

371 2678-2685.

372 Donath, L., Faude, O., Lichtenstein, E., Nüesch, C., Mündermann, A., 2016. Validity and
373 reliability of a portable gait analysis system for measuring spatiotemporal gait
374 characteristics: comparison to an instrumented treadmill. 13, 1.

375 Favre, J., Jolles, B.M., Aissaoui, R., Aminian, K., 2008. Ambulatory measurement of 3D knee
376 joint angle. 41, 1029-1035.

377 Fellin, R.E., Rose, W.C., Royer, T.D., Davis, I.S., 2010. Comparison of methods for
378 kinematic identification of footstrike and toe-off during overground and treadmill
379 running. 13, 646-650.

380 Ferrari, A., Cutti, A.G., Cappello, A., 2010a. A new formulation of the coefficient of multiple
381 correlation to assess the similarity of waveforms measured synchronously by different
382 motion analysis protocols. 31, 540-542.

383 Ferrari, A., Cutti, A.G., Garofalo, P., Raggi, M., Heijboer, M., Cappello, A., Davalli, A.,
384 2010b. First in vivo assessment of “Outwalk”: a novel protocol for clinical gait
385 analysis based on inertial and magnetic sensors. 48, 1-15.

386 Fleiss, J.L., 1986. Design and analysis of clinical experiments. John Wiley & Sons, NewYork.

387 Hamacher, D., Hamacher, D., Taylor, W.R., Singh, N.B., Schega, L., 2014. Towards clinical
388 application: repetitive sensor position re-calibration for improved reliability of gait
389 parameters. Gait Posture 39, 1146-1148.

390 Jaysrichai, T., Suputtitada, A., Khovidhungij, W., 2015. Mobile sensor application for
391 kinematic detection of the knees. 39, 599-608.

392 Kadaba, M.P., Ramakrishnan, H.K., Wootten, M.E., 1990. Measurement of lower extremity
393 kinematics during level walking. Journal of Orthopaedic Research 8, 383-392.

394 McGinley, J.L., Baker, R., Wolfe, R., Morris, M.E., 2009. The reliability of three-dimensional
395 kinematic gait measurements: a systematic review. 29, 360-369.

396 Meldrum, D., Shouldice, C., Conroy, R., Jones, K., Forward, M., 2014. Test–retest reliability
397 of three dimensional gait analysis: Including a novel approach to visualising
398 agreement of gait cycle waveforms with Bland and Altman plots. 39, 265-271.

399 Picerno, P., Cereatti, A., Cappozzo, A., 2008. Joint kinematics estimate using wearable
400 inertial and magnetic sensing modules. 28, 588-595.

401 Schwesig, R., Kauert, R., Wust, S., Becker, S., Leuchte, S., 2010. Reliabilitätsstudie zum
402 Ganganalysesystem RehaWatch/Reliability of the novel gait analysis system
403 RehaWatch. 55, 109-115.

404 Sprager, S., Juric, M.B., 2015. Inertial sensor-based gait recognition: a review. 15, 22089-
405 22127.

406 Takeda, R., Tadano, S., Natorigawa, A., Todoh, M., Yoshinari, S., 2009. Gait posture
407 estimation using wearable acceleration and gyro sensors. 42, 2486-2494.

408

409

Table 1: Root mean square error (RMSE) (1 standard deviation) between the kinematic waveform data measured by the RehaGait[®] and the reference system without and with offset correction, respectively and within the two sessions measured with the RehaGait[®] system for treadmill walking and running

	<i>Between RehaGait[®] and Vicon without offset correction</i>	<i>Between RehaGait[®] and Vicon with offset correction</i>	<i>Within RehaGait[®]</i>
<i>Walking</i>			
RMSE ankle	4.5 (2.1)	2.5 (0.9)	2.7 (1.7)
RMSE knee	7.6 (2.6)	5.0 (1.7)	3.1 (1.8)
RMSE hip	9.6 (3.0)	3.3 (0.8)	3.0 (2.5)
<i>Running</i>			
RMSE ankle	17.7 (5.4)	5.4 (3.6)	6.7 (4.1)
RMSE knee	17.9 (4.4)	7.8 (3.5)	5.3 (3.1)
RMSE hip	27.6 (3.2)	5.3 (2.2)	3.8 (2.4)

Table 2: Root mean square error of the discrete parameters between the RehaGait[®] and Vicon[®] system and between the test and re-test measurement with the RehaGait[®] system.

	<i>Walking</i>		<i>Running</i>	
	<i>Between RehaGait[®] and Vicon[®]</i>	<i>Within RehaGait[®]</i>	<i>Between RehaGait[®] and Vicon[®]</i>	<i>Within RehaGait[®]</i>
Ankle angle at initial contact	4.2	2.5	14.4	6.1
first minimal ankle angle	5.4	0.6	17.5	2.1
Maximal ankle angle	4.6	2.0	19.1	3.7
second minimal ankle angle	5.2	3.2	18.5	10.1
Ankle dorsiflexion range of motion	4.4	1.8	5.3	2.8
Ankle plantarflexion range of motion	4.0	2.6	7.1	10.4
Knee angle at initial contact	9.9	0.5	19.3	1.4
first maximal knee angle	10.1	3.3	20.0	5.4
Minimal knee angle	5.3	3.6	13.2	4.9
second maximal knee angle	7.1	4.3	19.8	8.8
Knee range of motion (first half stride)	3.7	3.1	5.7	3.9
Knee range of motion (second half stride)	8.4	4.1	7.6	9.1
Hip angle at initial contact	14.6	4.1	36.1	3.5
first maximal hip angle	12.8	3.5	33.2	2.7
Minimal hip angle	6.0	3.9	25.7	5.3
second maximal hip angle	9.8	3.7	25.1	3.8
Hip range of motion (first half stride)	7.6	2.3	8.6	4.0
Hip range of motion (second half stride)	4.6	1.9	4.2	3.9

Table 3: Comparison of discrete parameters during walking between the RehaGait system and the reference system (positive angles represent ankle dorsiflexion, knee flexion and hip flexion)

	RehaGait [®] 1	RehaGait [®] 2	Vicon [®]	<i>P</i> value (between systems) ^a	<i>P</i> value (within RehaGait [®]) ^b
	Mean (SD)	Mean (SD)	Mean (SD)		
Ankle angle at initial contact	7.4 (2.1)	7.0 (2.5)	8.7 (3.6)	.722	0.439
first minimal ankle angle	-1.3 (0.9)	-1.5 (0.8)	2.8 (3.6)	<0.001	0.132
Maximal ankle angle	15.9 (3.5)	15.8 (3.4)	16.6 (3.3)	0.446	0.796
second minimal ankle angle	-14.5 (4.8)	-16.2 (5.4)	-11.3 (4.3)	0.002	0.011
Ankle dorsiflexion range of motion	17.2 (3.5)	17.2 (3.5)	13.9 (3.3)	<0.001	0.848
Ankle plantarflexion range of motion	30.3 (3.4)	31.9 (4.1)	27.9 (4.4)	0.001	0.004
Knee angle at initial contact	-1.2 (0.5)	-1.4 (0.5)	7.3 (5.2)	<0.001	0.113
first maximal knee angle	17.2 (3.2)	18.1 (2.5)	25.2 (7.5)	<0.001	0.247
Minimal knee angle	4.9 (3.7)	7.2 (3.6)	6.8 (6.0)	0.236	0.002
second maximal knee angle	68.7 (5.2)	69.8 (3.8)	68.3 (7.1)	0.909	0.245
Knee range of motion (first half stride)	18.6 (3.3)	19.6 (2.3)	20.3 (4.8)	0.029	0.137
Knee range of motion (second half stride)	70.0 (5.2)	71.3 (3.7)	63.4 (5.5)	<0.001	0.161
Hip angle at initial contact	22.9 (3.2)	23.4 (4.5)	37.1 (3.0)	<0.001	0.576
first maximal hip angle	25.5 (3.4)	26.5 (4.6)	37.7 (3.4)	<0.001	0.200
Minimal hip angle	-12.0 (4.9)	-11.1 (3.6)	-7.2 (4.7)	<0.001	0.325
second maximal hip angle	29.8 (3.8)	30.1 (5.2)	38.9 (3.1)	<0.001	0.721
Hip range of motion (first half stride)	37.4 (3.6)	37.6 (3.9)	44.9 (3.6)	<0.001	0.779
Hip range of motion (second half stride)	41.8 (4.0)	41.2 (4.1)	46.1 (3.5)	<0.001	0.183

^a: general linear model with factors time and system

^b: least square difference test

Table 4: Comparison of discrete parameters during running between the RehaGait system and the reference system (positive angles represent ankle dorsiflexion, knee flexion and hip flexion).

	RehaGait® 1	RehaGait® 2	Vicon®	<i>P</i> value (between systems) ^a	<i>P</i> value (within RehaGait) ^b
	<i>Mean (SD)</i>	<i>Mean (SD)</i>	<i>Mean (SD)</i>		
Ankle angle at initial contact	1.1 (8.4)	1.1 (5.7)	13.6 (4.6)	<0.001	0.663
first minimal ankle angle	-6.5 (4.1)	-5.5 (2.7)	10.8 (3.9)	<0.001	0.316
Maximal ankle angle	14.9 (4.1)	14.8 (2.7)	33.2 (5.4)	<0.001	0.942
second minimal ankle angle	-36.9 (7.5)	-34.2 (9.1)	-19.5 (4.3)	<0.001	0.163
Ankle dorsiflexion range of motion	21.4 (4.7)	20.4 (3.4)	22.4 (5.2)	0.092	0.515
Ankle plantarflexion range of motion	51.8 (7.8)	49.0 (8.9)	52.7 (7.0)	0.001	0.186
Knee angle at initial contact	-2.0 (1.3)	-1.6 (0.8)	16.6 (5.6)	<0.001	0.196
first maximal knee angle	29.8 (4.6)	31.6 (4.0)	49.2 (5.0)	<0.001	0.145
Minimal knee angle	1.7 (3.4)	3.6 (4.1)	14.0 (6.6)	<0.001	0.084
second maximal knee angle	78.5 (9.9)	81.0 (10.2)	96.6 (10.2)	<0.001	0.212
Knee range of motion (first half stride)	31.4 (3.9)	30.9 (3.7)	36.1 (4.9)	<0.001	0.621
Knee range of motion (second half stride)	81.2 (10.0)	82.9 (10.4)	83.6 (9.8)	0.292	0.414
Hip angle at initial contact	10.0 (3.0)	11.7 (4.3)	45.9 (3.3)	<0.001	0.025
first maximal hip angle	13.2 (2.7)	14.3 (4.3)	46.2 (3.6)	<0.001	0.088
Minimal hip angle	-30.2 (5.7)	-27.6 (5.2)	-4.9 (4.5)	<0.001	0.024
second maximal hip angle	25.5 (3.5)	27.3 (4.5)	50.4 (3.3)	<0.001	0.032
Hip range of motion (first half stride)	43.4 (5.1)	41.8 (4.3)	51.0 (4.8)	<0.001	0.078
Hip range of motion (second half stride)	55.7 (6.9)	54.9 (7.2)	55.2 (5.7)	0.206	0.370

^a: general linear model with factors time and system

^b: least square difference test

Figure Captions

Figure 1: A) Inertial sensor with elastic strap; B) Placement of the inertial sensors laterally on the foot (below lateral malleolus) and the shank (lower third); C) Dorsal view of the placement of the inertial sensors on the foot, shank, thigh (middle) and sacrum.

Figure 2: Comparison between mean joint angles of the 20 subjects during walking (left column) and running (right column) measured by the RehaGait[®] (dashed line) and the reference system (solid line). The grey area indicates the mean \pm 95% confidence interval difference between the two systems. For each joint and conditions the coefficient of multiple correlation (CMC) is indicated in the respective graph.

Figure 3: Bland-Altman plots for the ranges of motion (ROM) of the ankle, knee and hip joint during the stance phase for the test re-test comparison of walking (left column) and running (right column). Each graph presents the mean difference (solid line) and 1.96-fold standard deviation of the difference (dashed lines) between the two measurements. Intraclass correlation coefficients (ICC) between the measurements are indicated in the titles of each angle.

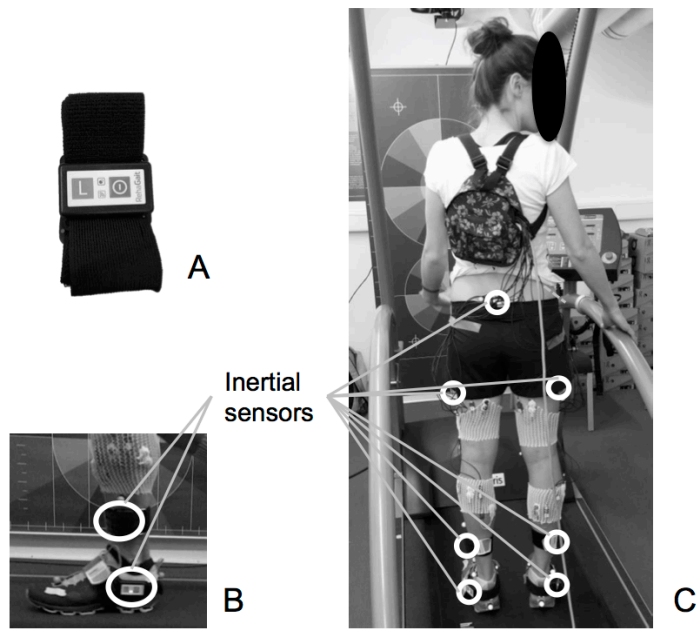


Figure 1

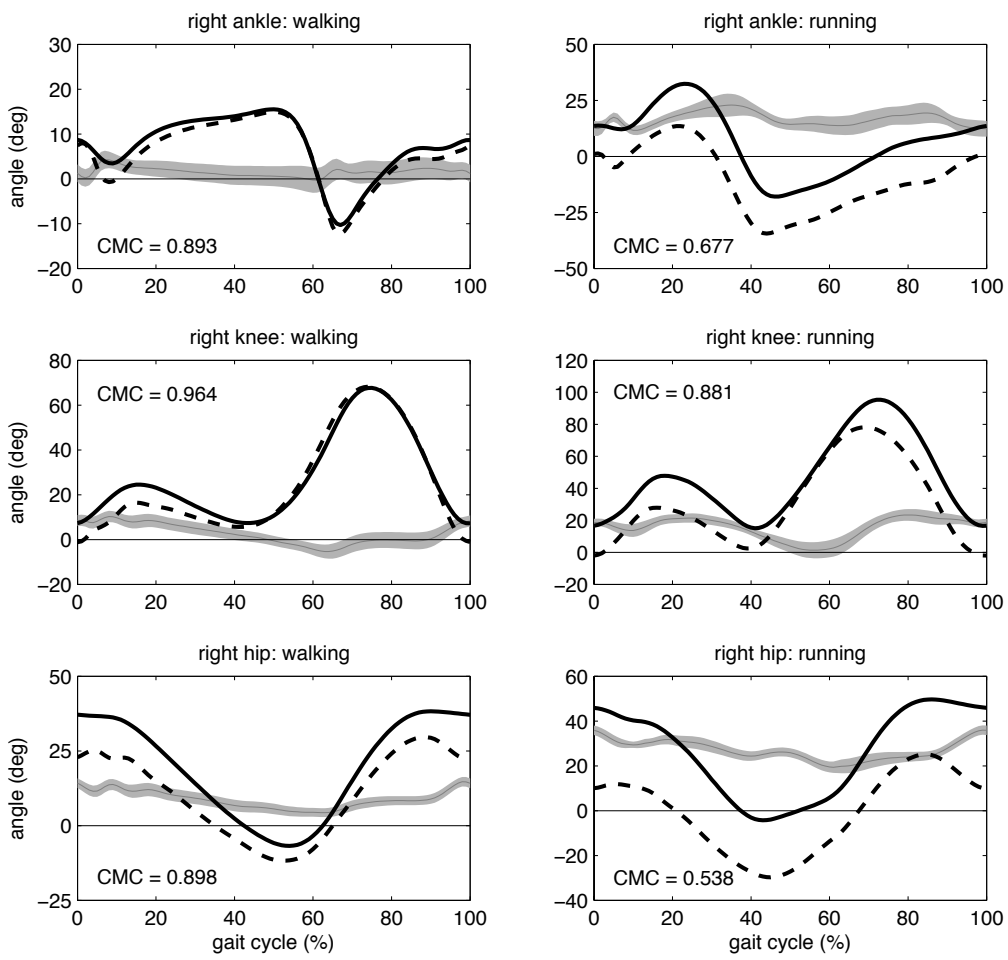


Figure 2

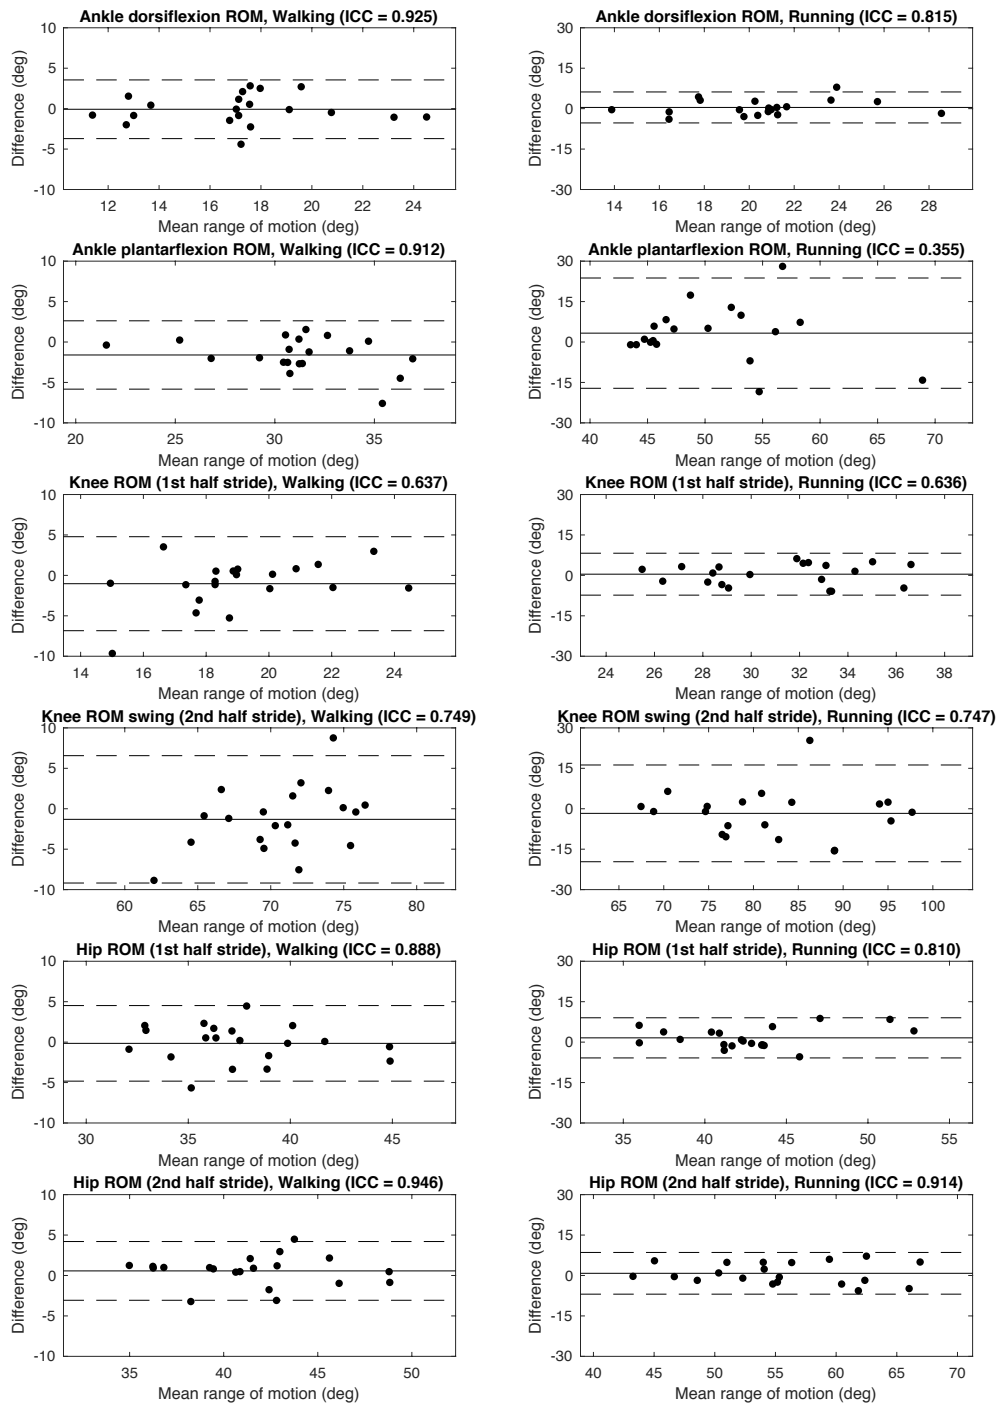


Figure 3